

# Pulse Oximeter JPD-500G

## FCC statement

This device complies with Part 15 of the FCC Rules. Operation is subject to the following two conditions :

- (1) This device may not cause harmful interference.
- (2) This device must accept any interference received, including interference that may cause undesired operation.

NOTE: This equipment has been tested and found to comply with the limits for a Class B digital device, pursuant to Part 15 of the FCC Rules. These limits are designed to provide reasonable protection against harmful interference in a residential installation. This equipment generates, uses and can radiate radio frequency energy and, if not installed and used in accordance with the instructions, may cause harmful interference to radio communications.

However, there is no guarantee that interference will not occur in a particular installation. If this equipment does cause harmful interference to radio or television reception, which can be determined by turning the equipment off and on, the user is encouraged to try to correct the interference by one or more of the following measures:

- ☒ Reorient or relocate the receiving antenna.
- ☒ Increase the separation between the equipment and receiver.
- ☒ Connect the equipment into an outlet on a circuit different from that to which the receiver is connected.
- ☒ Consult the dealer or an experienced radio/TV technician for help.

**Warning:** Changes or modifications to this unit not expressly approved by the party responsible for compliance could void the user's authority to operate the equipment.

## Precautions

- Do not attempt to repair the Oximeter unless you are professional engineers. Only professionals with maintenance qualification are allowed to perform interior maintenance as necessary.
  - Change the contact position between the Oximeter probe and the finger periodically if you are monitoring your SpO2 levels and pulse rate for more than 2 hours.
  - Stop immediately if you have broken skin or the blood circulation of your finger is affected during prolonged use.
  - This product is not designed to be used by newborn babies.
- Seek for medical care if the measured value goes beyond the normal range and you are sure that the instrument is not malfunctioning.
- The pulse oximeter uses infrared light (invisible to your eyes) to measure your SpO2 levels. Hence, please do not stare at the light-emitting components of the Oximeter, as that could cause harm and/or potentially blind your eyes.
  - This pulse oximeter is not a medical device and is not intended to diagnose or treat any medical condition or disease. It is intended for non-medical use in healthy people to monitor their pulse and blood oxygen levels during sports and/or aviation only.

People who need SpO2 and pulse rate measurements because of a medical condition should not use the oximeter and should consult with their physician.

- For details about clinical limitations and contraindications, please carefully consult relevant medical literatures.

The following factors may affect the accuracy of the measurement:

- The Oximeter is used in an environment involving high-frequency devices, such as high-frequency electric knives and CT apparatuses.
- Ambient light intensity is too bright. Hence, please avoid direct exposure to strong light (such as beams from operating lamps or sunlight) during measurement.
- The probe of the Oximeter is placed on the same arm that a blood pressure cuff arterial duct or intravenous injection.
- The user suffers from hypotension, severe vascular atrophy, severe anemia, or low oxygen.
- The user is in sudden cardiac arrest or shock state.
- The user is wearing nail polish or artificial nails.

## Warnings

**Warning:** Do not use the Oximeter in an environment with any flammable gases, flammable anesthetic, or other flammable substances.

**Warning:** Keep unit and lanyard away from children as the included lanyard may present an entanglement or choking hazard to small children. Adult supervision required; never leave children unattended with unit or lanyard

**Warning:** Do not throw the batteries into fire, as that could cause an explosion.

**Warning:** Do not attempt to charge the included batteries, as that could cause leakage, fire disaster, or even explosion. Dispose the used batteries in accordance to the local laws and regulations.

**Warning:** Do not use the Oximeter in an MRI or CT environment.

**Warning:** Caution: Do not operate the Oximeter if it is wet. Avoid moving the oximeter from a cold to a hot and humid environment.

**Warning:** Install the batteries properly before powering on the Oximeter for normal use. Please remove the batteries if you are not planning to use the Oximeter for a long time.

**Warning:** Close the battery cover when the instrument is in use.

## Symbols

| Symbol  | Meaning  |
|---|--|
|  | Type BF applied part   |
|  | Caution: Please see this manual.   |
| %SpO2   | Symbol of oxygen saturation  |
| bpmPR   | Symbol of pulse rate   |
|  | No SpO2 alarms.  |
|  | When end users abandon this product, they must send the product to the collection place for recycling. |

## Overview

Oxygen saturation is the percentage of oxyhemoglobin (HbO2) that is combined with oxygen against all combinable hemoglobin (Hb). It is an important physiological parameter involved in respiration and circulation. The oxygen

saturation of arterial blood in a normal human body is 98%. Oxygen saturation is an important indicator of the oxygen condition in the human body. In general, the normal values of oxygen saturation shall not be lower than 94%. If the measured value of oxygen saturation is lower than 94%, an insufficient supply of oxygen is considered.

The pulse rate is the number of pulse beats per minute. Normally, the pulse rate is consistent with the heart rate. In general, the pulse rate of every person is 60 to 90 beats per minute.

The Perfusion Index (PI) usually reflects the limb perfusion status of an examined patient, and shows the detection precision of the instrument as well; that is, examination can still be performed even in the low or weak perfusion condition. The PI of a normal human body is 3% or greater.


## Working Principles and Usage

Based on full digital technology, the Finger Pulse Oximeter non-invasively measures the actual content (oxygen saturation) of oxyhemoglobin (HbO2) in arterial blood using the optical transmittance method.

The Finger Pulse Oximeter measures the blood oxygen saturation and pulse rate of a human body via finger artery. It is applicable to a wide range of fields, such as families, hospitals (including operation rooms of the departments of internal medicine and surgery, the department of anesthesiology, the department of paediatrics, and intensive care rooms), oxygen bars, social medical care institutions, and sports & health. Use this instrument for measurement before or after sports.


You are not advised to use this instrument during sports activities. Do not use it for continuous care for patients.

## Schematic Diagram of Display

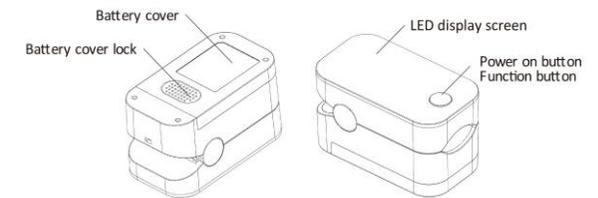

## Schematic Diagram of Display

The following figure shows the information display on the LED screen of the Oximeter in normal detection state:

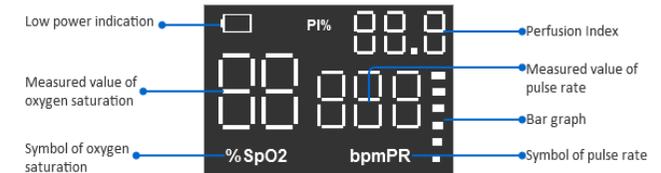

## Power-On button/Function Button Operations

Press the power-on/function button to turn on the oximeter. Once it is turned on, simply press or hold the button to perform corresponding operations.

Press: Press the button for less than 0.5 seconds.  
 Hold: Press the button for more than 0.5 seconds.

### Brightness Setting

Hold the power-on button while the oximeter is in powered-on state, then the oximeter shows a brightness setting interface (as "Interface 1" below shows, "br" represents brightness). Hold the button to adjust brightness. There are 3 brightness settings (1, 2, 3). 3 is the brightest.



Interface 1

### Alarm Setting

After setting the brightness, press the power-on button to enter the alarm setting interface (as "Interface 2" below shows, "AL" represents alarm). Then hold the button to set "AL" to on or off. When "AL" is set to on and the measured values of the blood oxygen saturation and pulse rate go beyond the upper limit or lower limit, the oximeter will beep to alarm.




Interface 2

### Alert Range Setting

When "AL" is set to on, you can set the upper limit and lower limit of SpO2 Alert and PR Alert. Press it to switch an option (SpO2 upper limit, SpO2 lower limit, PR upper limit and PR lower limit). Hold the power-on button to adjust the limits. (as "Interface 3, 4, 5, 6" below show, "Hi" represents upper limit, "Lo" represents lower limit).




Interface 3



Interface 4



Interface 5



Interface 6

### Operation Guide

Stick one finger completely into the finger chamber of the oximeter. The fingernail should be facing upward. Release the clip and press the power-on button to power on the pulse oximeter.




⚠️ If you do not insert your finger completely into the chamber, measurement will be inaccurate.

⚠️ To keep your finger still during measurement. It is also not advisable to use this instrument during sports activities as movement may lead to inaccuracies. Once the

reading stabilizes, read the measured values of oxygen saturation and pulse rate on the screen.

NOTE: The oximeter will automatically shut down 10 seconds after you remove your finger.

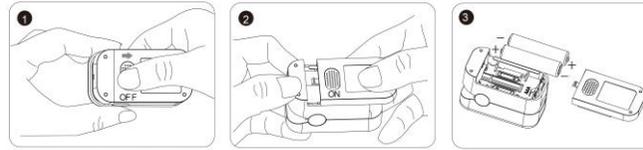

⚠️ Replace the batteries when the batteries run out of power and the symbol (🔋) flickers on the screen.

Install the two AAA dry batteries into the battery slot according to polarity indication, and mount the battery cover.

### Cleaning

Power off the instrument and remove the batteries before cleaning. Ensure that the appearance of the instrument is neat, dust-free, and dirt-free. Clean the outer surface of the instrument (including the LED screen) using a piece of dry soft cloth dipped with 75% medical alcohol.

**Caution:** Avoid liquid flowing into the instrument during cleaning.

**Caution:** Do not immerse any part of the instrument into any liquid.

### Disinfection

Before measurement with the instrument, wipe the rubber finger pad using a piece of dry soft cloth dipped with 75% medical alcohol. Clean the finger to be measured using the medical alcohol for disinfection purposes before and after use.

⚠️ Do not disinfect the instrument by means of high-temperature/high-pressure or gas disinfection.

### Maintenance

- Remove the batteries from the battery slot and properly store them if you do not plan to use the Oximeter for a long period of time.
- Avoid using the Oximeter in an environment with inflammable gases or using it in an environment where the temperature or humidity is excessively high or low.
- Check the accuracy of the oxygen saturation and pulse rate readings by using an appropriate calibration apparatus.

### Technical Specifications

- Dimensions: 58.0 mm (Width) × 32.0 mm (Depth) × 32.9 mm (Height)  
Weight: 50.4 g (including two AAA dry batteries)
- Peak wavelength range of the light emitted from the probe: red light 663 nm ± 3; infrared light 900 nm ± 7.
- Maximum optical output power of the probe: 60 mW for infrared light (905 nm).
- Normal working condition

|                      |                             |
|----------------------|-----------------------------|
| Working Temperature  | 5°C to 40°C (41°F to 104°F) |
| Relative Humidity    | 15% to 80%, non-condensing  |
| Atmospheric Pressure | 70 kPa to 106 kPa           |

|               |          |
|---------------|----------|
| Rated Voltage | DC 3.0 V |
|---------------|----------|

### 5. Default values and conditions of alert

| Parameter         | Value  |
|-------------------|--|
| Oxygen saturation | Upper limit: 99<br>Lower limit: 94   |
| Pulse rate        | Upper limit: 130<br>Lower limit: 50  |
| Alert condition   | When the alert switch is on and the actual measured value goes beyond the preset alert parameter range, the Oximeter gives an alert sound. |

### 6. Technical parameters

| Parameter             | Value             |  |
|-----------------------|-------------------|--|
| Display range         | Oxygen saturation | 35% to 99%   |
|                       | Pulse rate        | 35 bpm to 250 bpm  |
| Resolution            | Oxygen saturation | 1%   |
|                       | Pulse rate        | 1 bpm  |
| Measurement precision | Oxygen saturation | ±2% (70% to 99%)<br>No requirement (≤ 69%)                       |
|                       | Pulse rate        | ±2 bpm   |
| Alert range           | Oxygen saturation | Upper limit: 50% to 100%<br>Lower limit: 50% to 100%             |
|                       | Pulse rate        | Upper limit: 35 bpm to 250 bpm<br>Lower limit: 35 bpm to 250 bpm |
| Alert error           | Oxygen saturation | ± 1% of the preset value   |
|                       | Pulse rate        | The greater of ±10% of the preset value and ±5 bpm               |
| PI                    | Weak PI           | Min. 0.3%  |

### Safety Type

Anti-electric-shock type: internal power supply device  
 Anti-electric-shock degree: Type BF applied part  
 Running mode: continuous working  
 Waterproof grade: IP22

### Storage and Transportation

Temperature : -10°C - 50°C (14°F - 122°F)  
 Relative humidity : 10%-93% (no condensation)  
 Atmospheric pressure : 50kPa-106 kPa.



Wellkang Ltd  
 Suite B, 29Harley Street, LONDON, W1G9QR, U.K.



Shenzhen Jumper Medical Equipment Co., Ltd  
 Address: D Building, No. 71, Xintian Road, Fuyong Street, Baoan, Shenzhen, Guangdong, China  
 E-mail: info@jumper-medical.com  
 Tel: +86-755-26692192, 26696279  
 Web: www.jumper-medical.com

**JUMPER**