


MANUAL

First15 Tourniquet

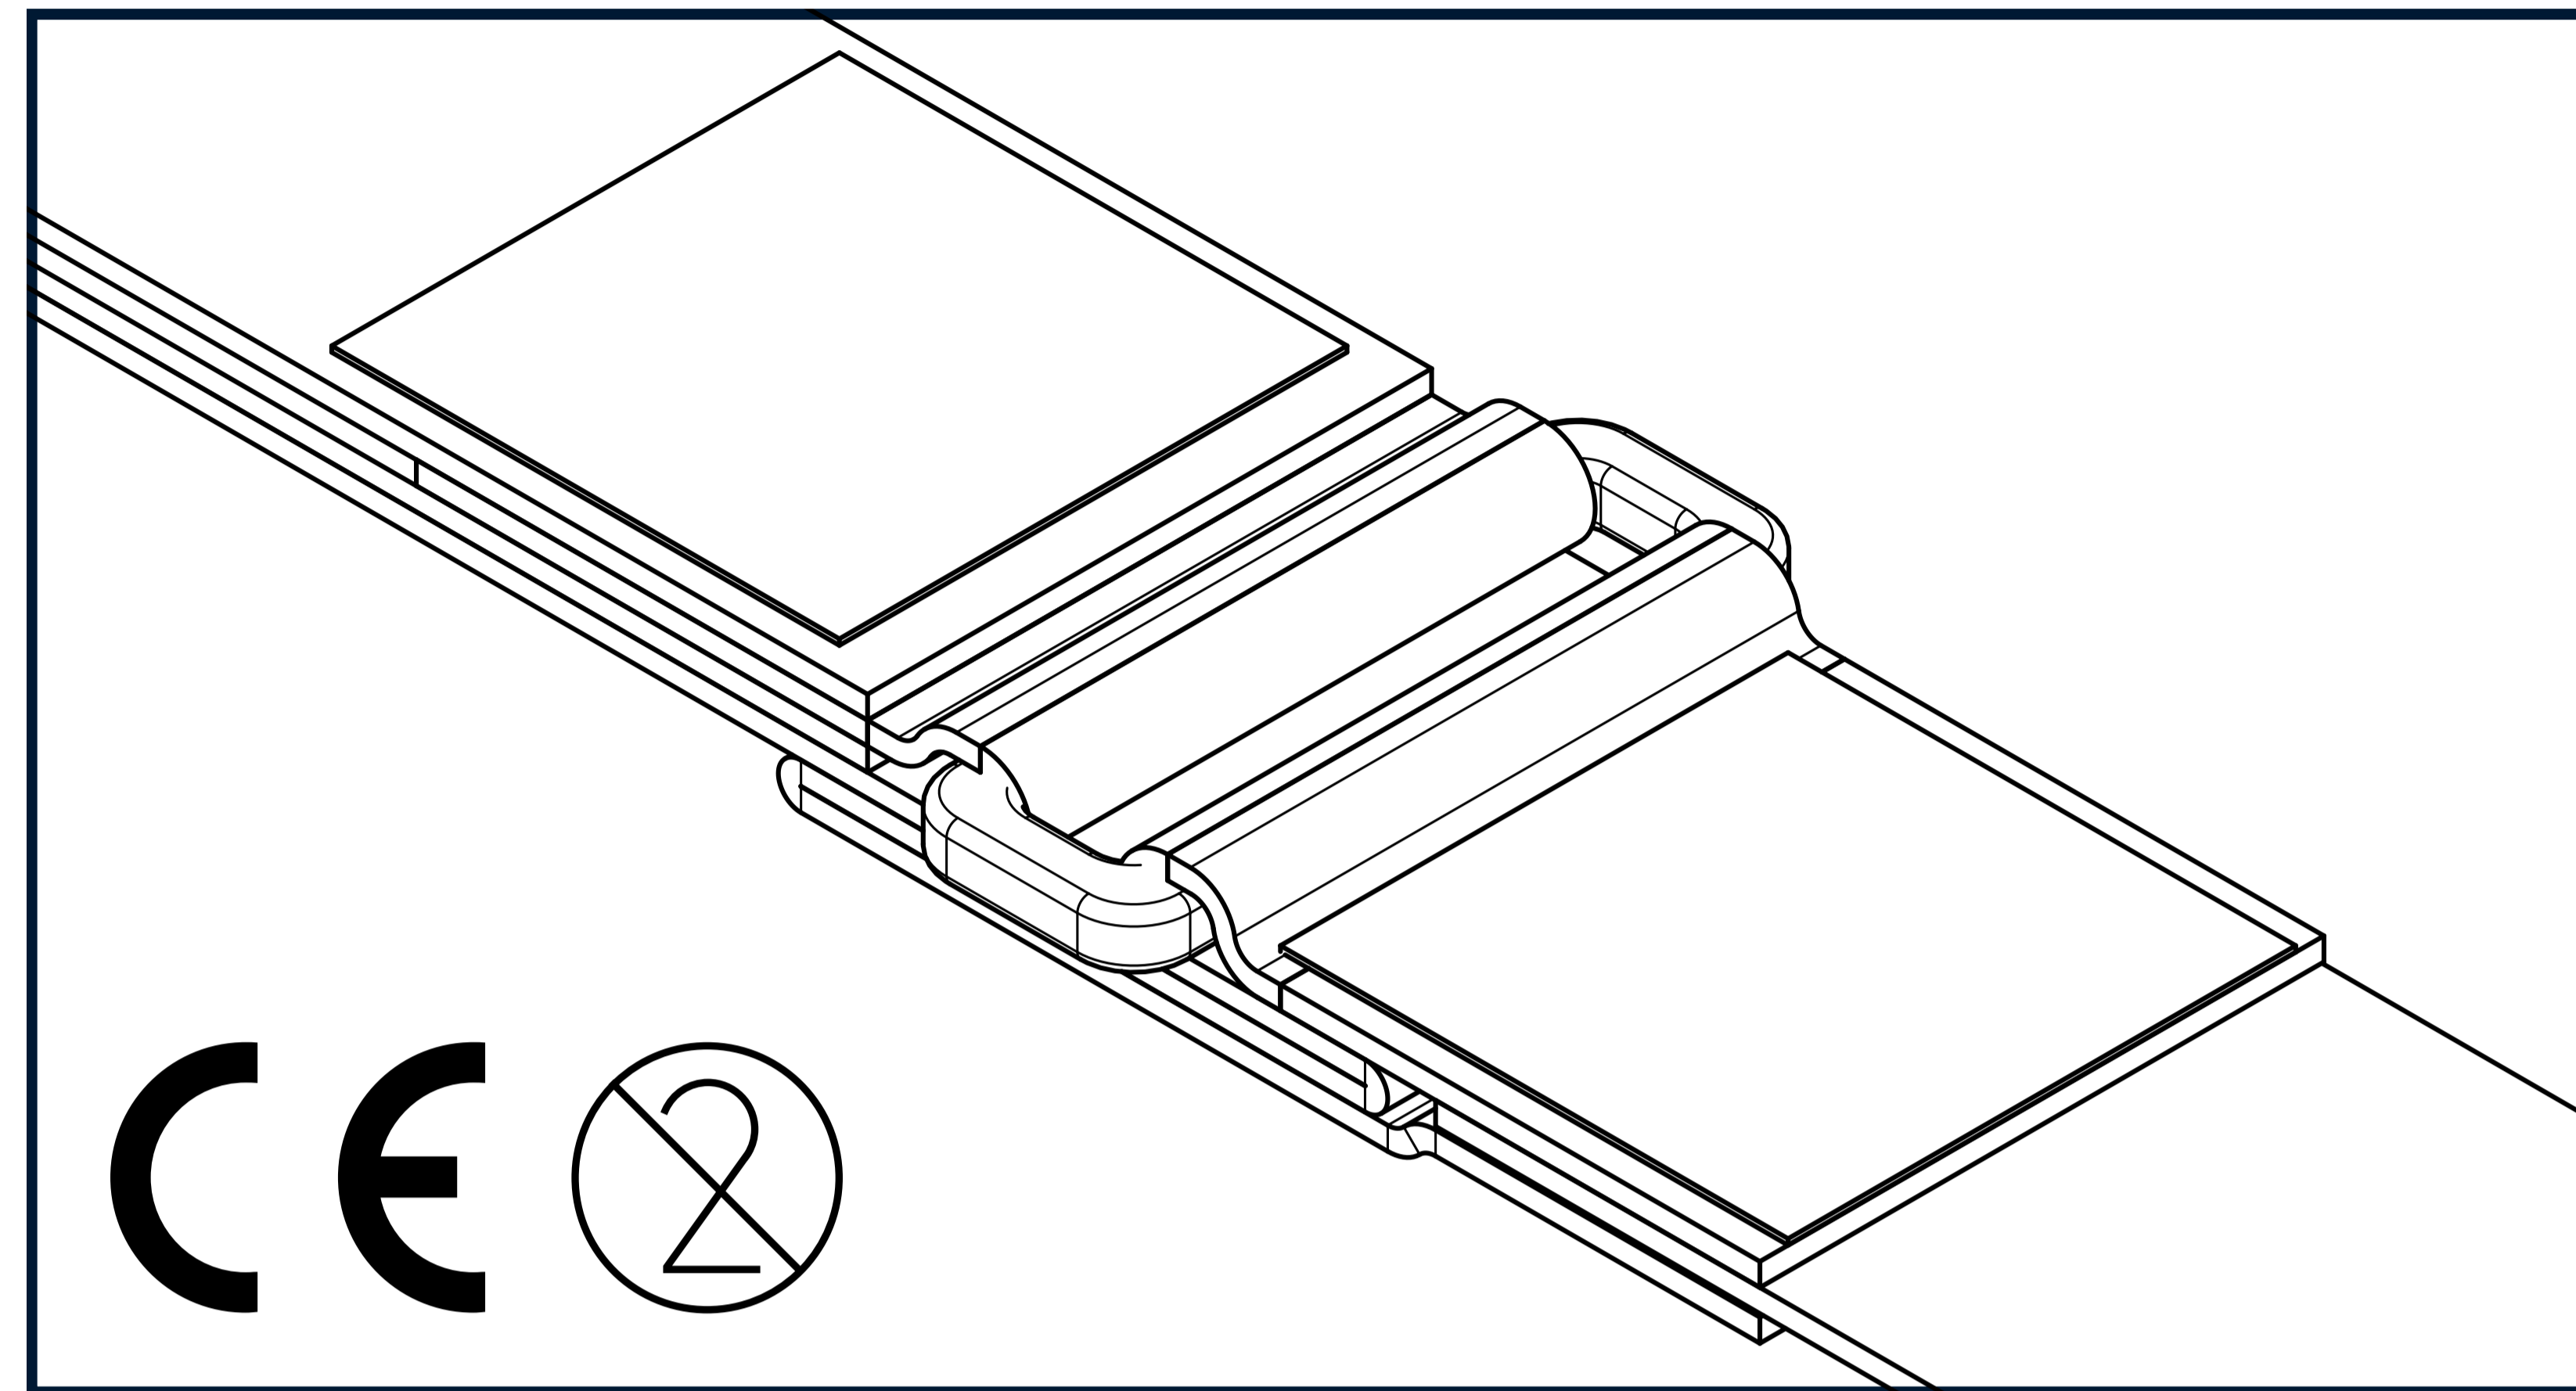

Limitation of liability.

First15 B.V. , its employees,agents,contractors,suppliers and distributors shall assume no liability for injury or damages resulting from the application and use of the First15 tourniquet.

The user assumes all risks of liability. The First15 Tourniquet should only be used as directed by medical authorities or under the supervision of a physician.

Report any incident involving this device to the manufacturer and the appropriate authority in the country or state where the user and or patient is located.


This product is a Class 1 medical device that may require specific training in its proper use. Please follow local or governmental guidelines regarding the use of this device

The use of a tourniquet is a last resort and it should only be used in a life threatening situation and when bleeding cannot be stopped.


FIRST15

First15 B.V. All rights reserved.
Laan van Kronenburg 14. 1183 AS, Amstelveen


For more information visit:
WWW.FIRST15.ONLINE

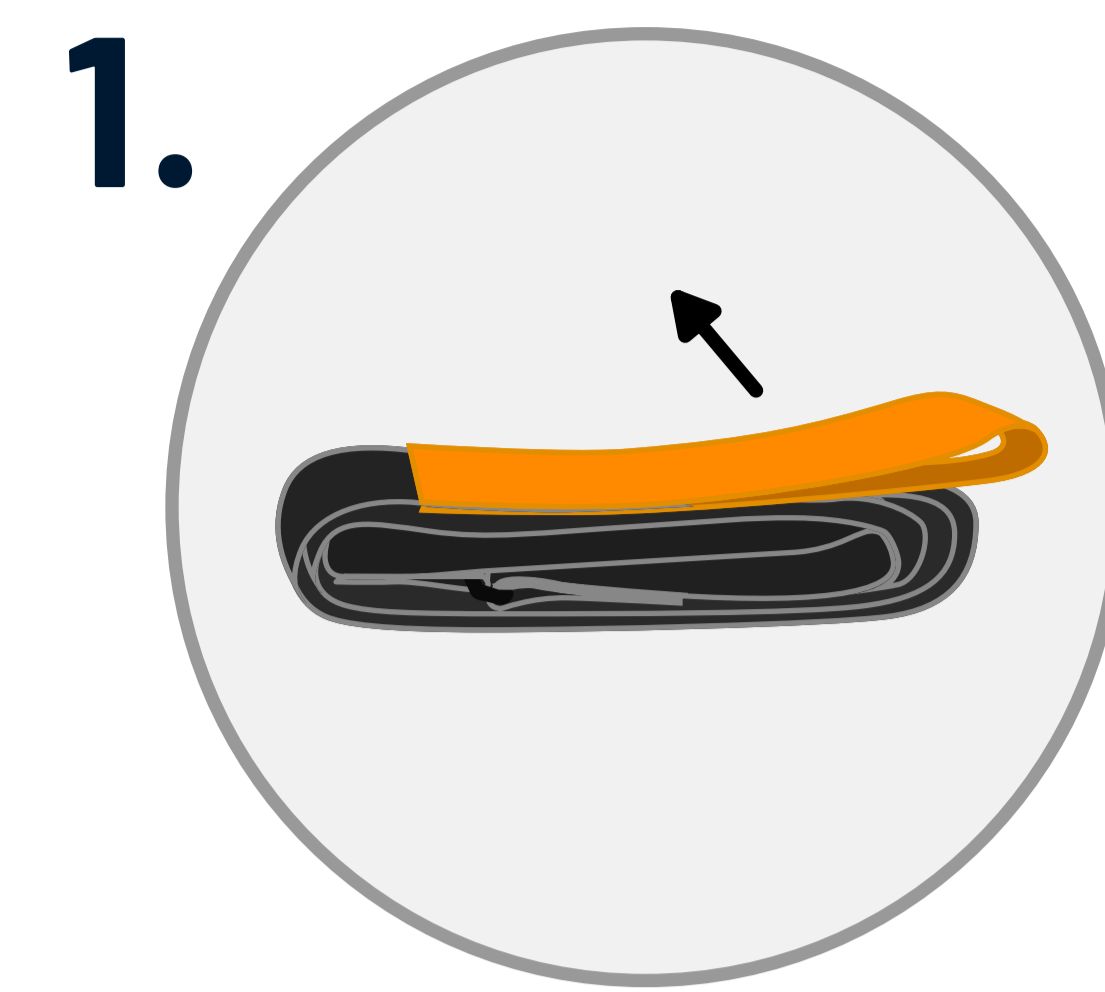

1. Open the package and unroll the tourniquet fully.

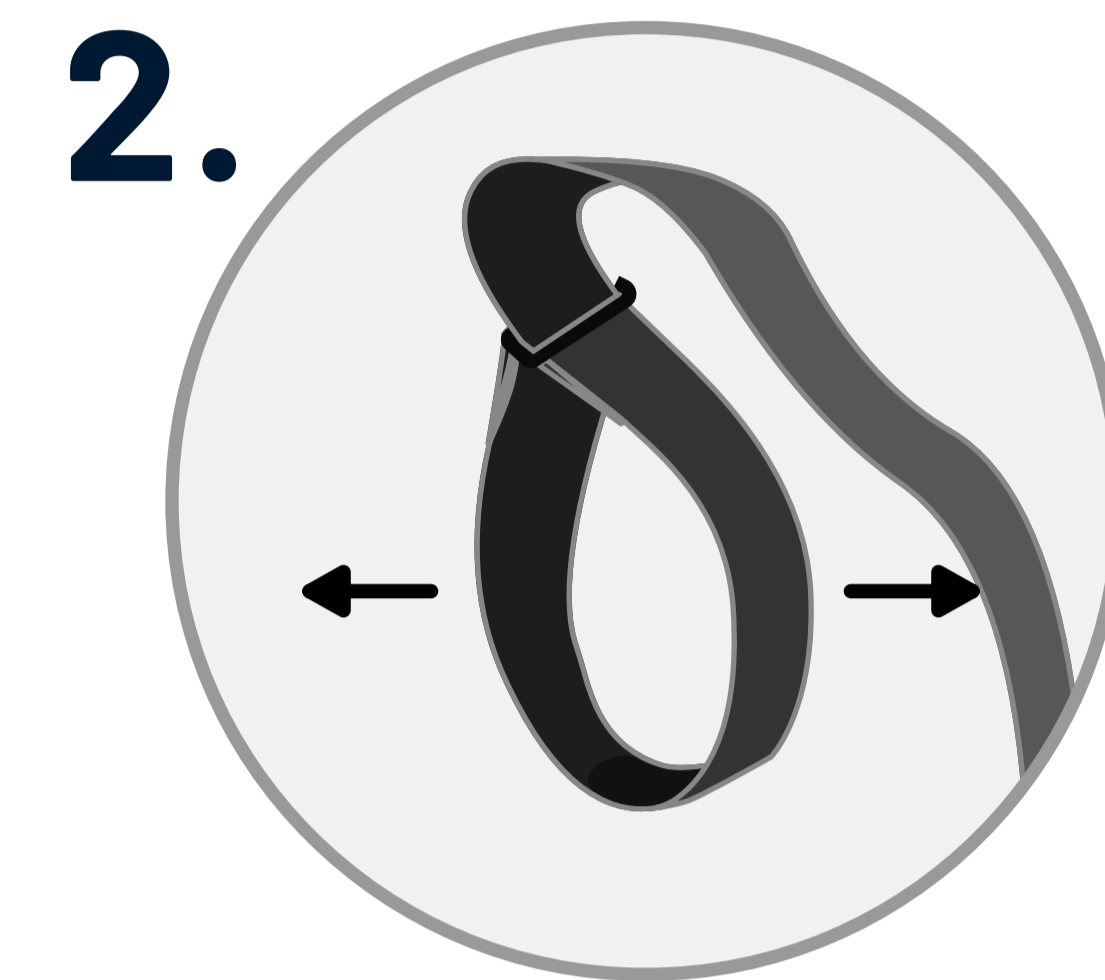

2. Widen the loop of het tourniquet so that it fits over the affected limb.

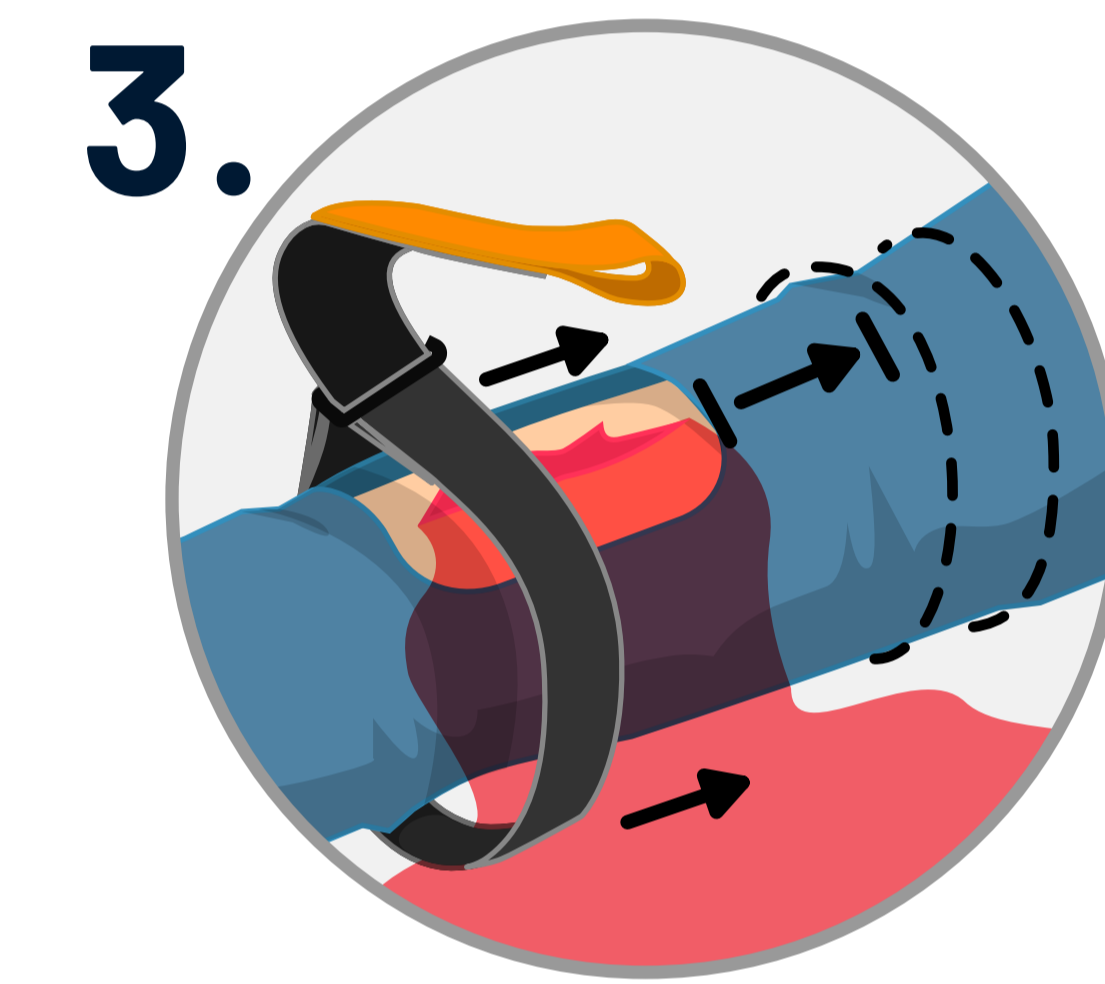



3. Slide the tourniquet over the affected limb, **above** the level of the bleeding.

3.1 Place the tourniquet at least **2 Inch / 5 cm** above the wound.

3.2 Apply the tourniquet to the **upper arm** or **thigh**.

! The tourniquet may only be applied to the upper arm or thigh.

✗ **Never** apply the tourniquet to a joint!

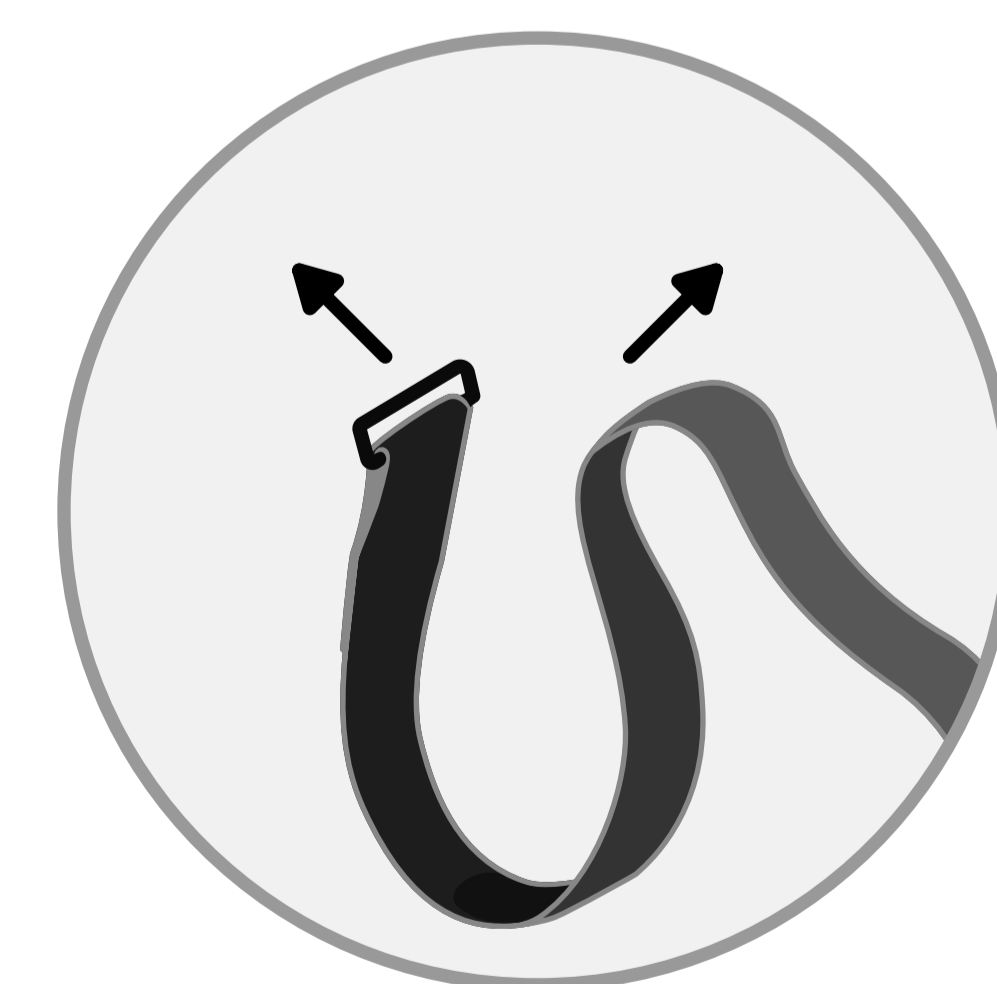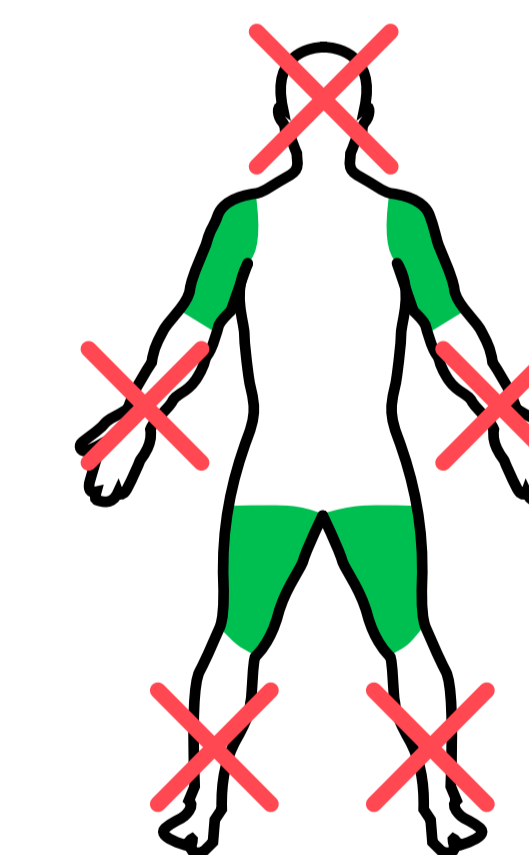


Loosen the tourniquet completely. Wrap it around the limb and secure it by putting the end through the buckle again.

CAUTION!

In case it is not possible to slide the loop around the leg or arm:



4. Pull the strap so the loop is tight around the limb.

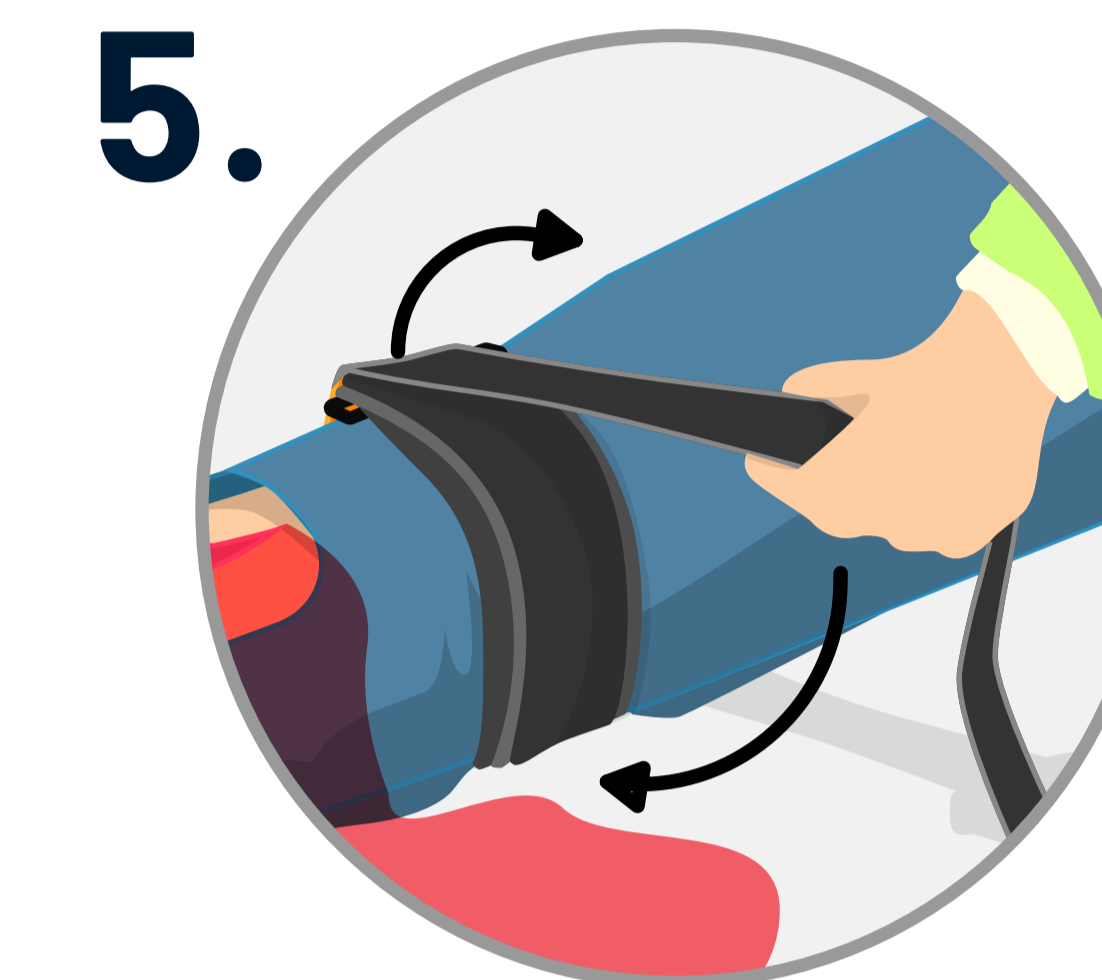

5. Wind the strap **as tightly as possible** around the limb while maintaining compression by pulling hard.

5.1 Use the entire length of the tourniquet.

! With each turn, check to see if the bleeding decreases.



6. On the final turn, use the handle to apply extra pressure and **secure** the tourniquet with the Velcro.

! The tourniquet is tight enough when the bleeding stops.



7. Check regularly that there is still **complete occlusion**.

! Periodically check to make sure there is still complete occlusion. Movement and changes in muscle tension can cause the tourniquet to loosen.

! This product is for single use only. (The product should not be used multiple times).