

# ImageView Help Manual

ImageView Help Manual .....	I
1 How to start?.....	1
1.1 How to Start ImageView? .....	1
1.2 How to start the camera? .....	1
2 Video window GUI.....	2
2.1 Video window GUI .....	2
2.2 How to close the video window?.....	3
3 Image window GUI.....	5
3.1 Image window GUI .....	5
3.2 How to close the image window?.....	6
4 UI toolbar.....	8
5 Camera Sidebar.....	10
5.1 Camera List group .....	10
5.2 Capture & Resolution group .....	10
5.3 Exposure & Gain group .....	10
5.4 White Balance group .....	11
5.5 Color Adjustment group .....	11
5.6 Frame Rate group .....	12
5.7 Flip group .....	12
5.8 Color/Gray group .....	12
5.9 Power Frequency group .....	12
5.10 Sampling group .....	13
5.11 Bit Depth group .....	13
5.12 ROI group .....	13
5.13 Histogram group .....	13
5.14 Dark Field Correction .....	14
5.15 Misc .....	14
5.16 Parameters group .....	15
6 File.....	16






## ImageView Help Contents

---

6.1 Open Image(O)•••		Ctrl+O .....	16
6.2 Open Video(V)•••		.....	18
6.3 Open Broadcast(C)•••		.....	19
6.4 Save(S)		Ctrl+S .....	19
6.5 Save As(A)•••		.....	20
6.5.1 Option for JPEG.....			21
6.5.2 Option for PNG.....			22
6.5.3 Option for TIF.....			22
6.5.4 Option for JPEG 2000 Stanndard, JPEG 2000 Codestream.....			23
6.5.5 Option for Digital Imaging and Communication in Medicine (*.dcm) .....			23
6.5.6 Option for the other formats .....			24
6.6 Batch Save(B)•••		.....	24
6.6.1 Batch Save for a) style image window .....			25
6.6.2 Batch Save for b), c) or d) style image window .....			25
6.7 Quick Save(Q)		CTRL+Q .....	26
6.8 Paste as New File(N)		.....	27
6.9 Twain: Select Device•••		.....	27
6.10 Twain: Acquire•••		.....	28
6.10.1 Introduction.....			28
6.10.2 Steps for Twain Acquire.....			28
6.11 Print Setup(R)•••		.....	29
6.12 Print Preview(V)•••		Ctrl+Shift+P .....	30
6.13 Print(P)•••		Ctrl+P.....	30
6.14 Recent Files .....			30
6.15 Exit(X) .....			31
7 Edit.....			32
7.1 Cut(T)		Ctrl+X.....	32
7.1.1 Cut for Objects.....			32

## ImageView Help Contents

---

7.1.2	Cut for Browse window selected files .....	32
7.2	Copy(C)  Ctrl+C .....	32
7.2.1	Copy the selected area on the background layer to the clipboard. .....	33
7.2.2	Copy object(s) on the measurement layer to the clipboard. .	33
7.2.3	Copy for Browse window selected files .....	34
7.3	Paste(P)  Ctrl+V .....	34
7.3.1	Paste for Objects.....	34
7.3.2	Paste for Browse window selected files .....	34
7.4	Paste Shortcut(S) .....	35
7.5	Delete(D)  Delete.....	35
7.5.1	For Browse Window file delete .....	35
7.5.2	For Video/Image Window Object delete .....	36
7.6	Image Select(S)  .....	36
7.7	Select All(A) Ctrl+A .....	37
7.7.1	Select all on the background layer .....	37
7.7.2	Select all objects over the background layer .....	37
7.7.3	Select all files in the Browse window .....	37
7.8	Select None(N) Ctrl+D.....	37
7.8.1	Select None for Background Layer .....	37
7.8.2	Select None for Objects .....	37
7.8.3	Select None for Browse window.....	37
8	View.....	38
8.1	Browse(B)  Ctrl+B .....	38
8.1.1	Open the Browse window.....	38
8.1.2	Browse window right mouse button context menu .....	38
8.2	Measurement Sheet(M) .....	39
8.2.1	Export Html .....	40
8.2.2	Auto Highlight.....	40
8.2.3	Settings••• .....	40
8.3	Sidebar .....	41

## ImageView Help Contents

---

8.3.1	Sidebar overview	41
8.3.2	Sidebar>Camera (C)	42
8.3.3	Sidebar>Folders (F)	43
8.3.4	Sidebar>Undo/Redo (U)	43
8.3.5	Sidebar>Layer (L)	44
8.3.6	Sidebar>Measurement (M)	44
8.4	Grid (G)	44
8.4.1	Settings (S) ••• 	44
8.4.2	Grids>No Grids (N)	45
8.4.3	Grids>Auto Grids (A)	45
8.4.4	Grids>Manual Grids (M)	45
8.4.5	Grids>Remove All Grids (R)	46
8.5	Best Fit (E) Num *	46
8.6	Actual Size (A) Num /	47
8.7	Full Screen (F)  ESC	47
8.8	Track (K) 	47
9	Browse	48
9.1	Sort (S)	48
9.1.1	Sort>Sort by Names (N)	48
9.1.2	Sort>Sort by Type (T)	48
9.1.3	Sort>Sort by Size (S)	48
9.1.4	Sort>Sort by Width (W)	48
9.1.5	Sort>Sort by Height (H)	48
9.1.6	Sort>Ascending (A) 	48
9.1.7	Sort>Descending (D) 	48
9.2	Icon (I)	49
9.2.1	Icon>Large Icons (L) 	49
9.2.2	Icon>Small Icons (S) 	49
9.3	Refresh (R)  F5	49
9.4	Properties (P) ••• 	49

## ImageView Help Contents

---

10	Setup.....		51
10.1	Start/Pause (U)		51
10.2	View Properties (V)•••	Shift+V	51
10.3	Video Overlay (O)•••		52
10.3.1	Video Overlay>Overlay.....		52
10.3.2	Video Overlay>Marker•••.....		52
10.4	Video Watermark (W)•••		54
10.5	Move Watermark (M)		55
10.5.1	Move to (W)•••.....		55
10.5.2	Move to zero.....		55
10.6	Rotate Watermark@		56
10.6.1	Rotate to (R)•••.....		56
10.6.2	Rotate to zero.....		56
10.7	Gray Calibration (G)•••		56
11	Capture.....		58
11.1	Capture Image (C)	 F8	58
11.2	Start Time-lapse (Auto Capture)•••		58
11.3	Start Record (V)•••	F9	59
11.4	Start Broadcast (B)•••		62
12	Image.....		64
12.1	Mode (M)		64
12.1.1	Color Quantize (Q)•••.....		64
12.1.2	Gray Scale (G).....		64
12.1.3	Contrast Preserving Decolorization@.....		64
12.2	Adjust (A)		65
12.2.1	Brightness/Contrast (A)•••.....		65
12.2.2	Color (O)•••.....		65
12.2.3	HMS•••.....		68
12.2.4	Curve (U)•••.....		68
12.2.5	Filter Color (F)•••.....		70
12.2.6	Extract Color (E)•••.....		71




## ImageView Help Contents

---

12.2.7	Invert (I) .....	71
12.2.8	Edge Preserving Smooth (S) ••• .....	71
12.2.9	Detail Enhance (D) ••• .....	72
12.2.10	Auto Level (L) .....	72
12.2.11	Auto Contrast (T) .....	73
12.3	Rotate (R) .....	74
12.3.1	90 (CW) .....	74
12.3.2	180 (CW) .....	74
12.3.3	270 (CW) .....	74
12.3.4	Arbitrary (A) ••• .....	74
12.3.5	Flip Horizontal (H)  .....	75
12.3.6	Flip Vertical (V)  .....	75
12.4	Crop (C)  Shift+C .....	75
12.5	Image Scale (S) •••  .....	76
12.6	Histogram (H) •••  Shift+H .....	77
12.7	Resolution (R) ••• .....	79
12.8	Mosaic (O) ••• .....	79
13	Process .....	82
13.1	Stitch (T) •••  Shift+T .....	82
13.1.1	Video Stitch .....	82
13.1.2	Image Stitch .....	85
13.1.3	Browse Window Stitch .....	87
13.2	High Dynamic Range (HDR) •••  .....	89
13.2.1	Browse window high dynamic range operation .....	89
13.2.2	Image window high dynamic range operation .....	89
13.3	EDF •••  Shift+F .....	91
13.3.1	Browse Window EDF .....	91
13.3.2	Image Window EDF .....	96
13.3.3	Video Window EDF  .....	98














## ImageView Help Contents

---

13.4 Deinterlace (A) .....	100
13.5 Color Composite (C) •••  .....	100
13.6 Segmentation & Count ••• .....	105
13.6.1 Watershed (W) ••• .....	106
13.6.2 OTSU Dark (D) ••• .....	109
13.6.3 OTSU Bright (B) ••• .....	109
13.6.4 RGB Histogram ••• .....	110
13.6.5 HSV Histogram ••• .....	113
13.6.6 Color Cubic (C) ••• .....	117
13.6.7 Split Objects (S) .....	122
13.6.8 Count Result (T) ••• .....	123
13.7 Denoise (D) .....	124
13.7.1 Adaptive Wiener Filter (A) .....	124
13.7.2 Bilateral Filter (B) ••• .....	125
13.7.3 Non Local Means (NLM) ••• .....	125
13.8 Sharpen (N) .....	126
13.8.1 USM (U) ••• .....	126
13.8.2 Laplacian Sharpen (L) .....	127
13.9 Color Toning (G) .....	128
13.9.1 Gamma (G) •••  .....	128
13.9.2 Histogram Equalization (Q) •••     Shift+Q .....	128
13.9.3 LCC® ••• .....	129
13.9.4 AMSR .....	130
13.10 Filter (I) •••     Shift+I .....	131
13.10.1 Image Enhance .....	131
13.10.2 Edge Enhance .....	134
13.10.3 Morphological .....	136
13.10.4 Kernel .....	138
13.11 Image Stacking (S) •••  .....	140
13.12 Line Profile (L) ••• .....	142
13.13 Surface Plot ••• .....	143
13.14 Pseudo Color (P) ••• .....	144

## ImageView Help Contents
















---

13.15	Range•••	Shift+R	145
13.16	Binary(B)•••	Shift+B	146
14	Layer		148
14.1	About layer		148
14.2	Organizing layers		148
14.3	Layers for non-destructive measurement and label		148
14.4	Layer Sidebar		148
14.5	Layer menu and layer sidebar page context menu		149
14.6	New(N)•••	 Ctrl+N	149
14.7	Remove(R)•••		149
14.8	Current(C)•••		150
14.9	Show/Hide(S)•••		150
14.10	Rename(E)•••		150
14.11	Export to Image(M)	F2	150
14.12	Export to Microsoft Excel•••	 F3	150
14.13	Export all to Microsoft Excel•••	 F4	150
15	Measurements		152
15.1	Object Select(S)		152
15.2	Angle(N)		153
15.2.1	Angle (3 Points)		153
15.2.2	Angle (4 Points)		153
15.3	Point(P)		154
15.4	Line(L)		155
15.4.1	Line>Arbitrary Line(A)		155












## ImageView Help Contents

---

15.4.2 Line> Horizontal Line(H)		155
15.4.3 Line> Vertical Line(V)		156
15.5 Parallel (R)		156
15.6 Two Parallels(O)		157
15.7 Vertical (V)		158
15.7.1 Vertical>Four Points.		158
15.7.2 Vertical>Three Points		159
15.8 Rectangle(T)		159
15.9 Ellipse(I)		160
15.10 Circle(C)		160
15.10.1 Circle>Center+Radius		160
15.10.2 Circle>Two Points		161
15.10.3 Circle>Three Points		161
15.11 Annulus (U)		162
15.12 Two Circles(W)		162
15.12.1 Two Circle>Center+Radius (R)		162
15.12.2 Two Circle>Three Points (3)		163



## ImageView Help Contents

---

15.13 Arc (A)		163
15.14 Text (X)		164
15.15 Polygon (G)		164
15.16 Curve (E)		165
15.16.1 Curve>Model 1		165
15.16.2 Curve>Model 2		166
15.17 Scale bar (B)		166
15.18 Arrow		167
15.19 Z Order (Z)		167
16 Options		169
16.1 Preferences (P) •••		169
16.1.1 Quick Save Page		169
16.1.2 File Page		170
16.1.3 Print Page		171
16.1.4 Grids Page		173
16.1.5 Cursor Page		173
16.1.6 Capture Page		174
16.1.7 Misc Page		175
16.2 Measurements (M) •••		176
16.2.1 General page		176
16.2.2 Length Unit page		177
16.2.3 Angle Unit page		178
16.2.4 Sheet page		179
16.2.5 Object page		179
16.3 Magnifications (F) •••		180
16.4 Calibrate (D) •••		181
16.5 Edit Dye List (E) •••		184




## ImageView Help Contents

---

16.6	Auto Correction(A) •••	185
17	Window.....	187
17.1	Close All(C)	187
17.2	Reset Window Layout(R)	188
17.3	Windows(W) ••• 	188
18	Help.....	190
18.1	Help Contents(H)  F1	190
18.2	About(A) •••	190

## 1 How to start?


### 1.1 How to Start ImageView?

1. Invoke the Windows metro start screen with keyboard button , locate [ImageView](#) and click it to start the application.
2. Click the [Start](#) button (At your screen bottom left corner) and a [Start](#) menu will bring up. Move your mouse over the menu and try to locate [ImageView](#) , click to start it.
1. Double click on the desktop icon "" (If installed) to start [ImageView](#);

### 1.2 How to start the camera?


[ImageView](#) will detect all of the cameras that your computer has installed (Here, it is [XXXXX](#), a 3.1M pixel USB3.0 CMOS camera) and will list all the camera names under the [Camera List](#) group on the [Camera Sidebar](#)

Click the [Camera Sidebar](#) (If it is not activated) and the [Camera List](#) to expand the [Camera List](#) group (if not expanded). Click the camera name (Here it is [XXXXX](#)) to start the video window and the camera will begin to stream the video. The video window will be associated with a name called "[Video \[XXXXX\]](#)" (i.e., its title bar name will be "[Video \[XXXXX\]](#)").



## 2 Video window GUI

### 2.1 Video window GUI

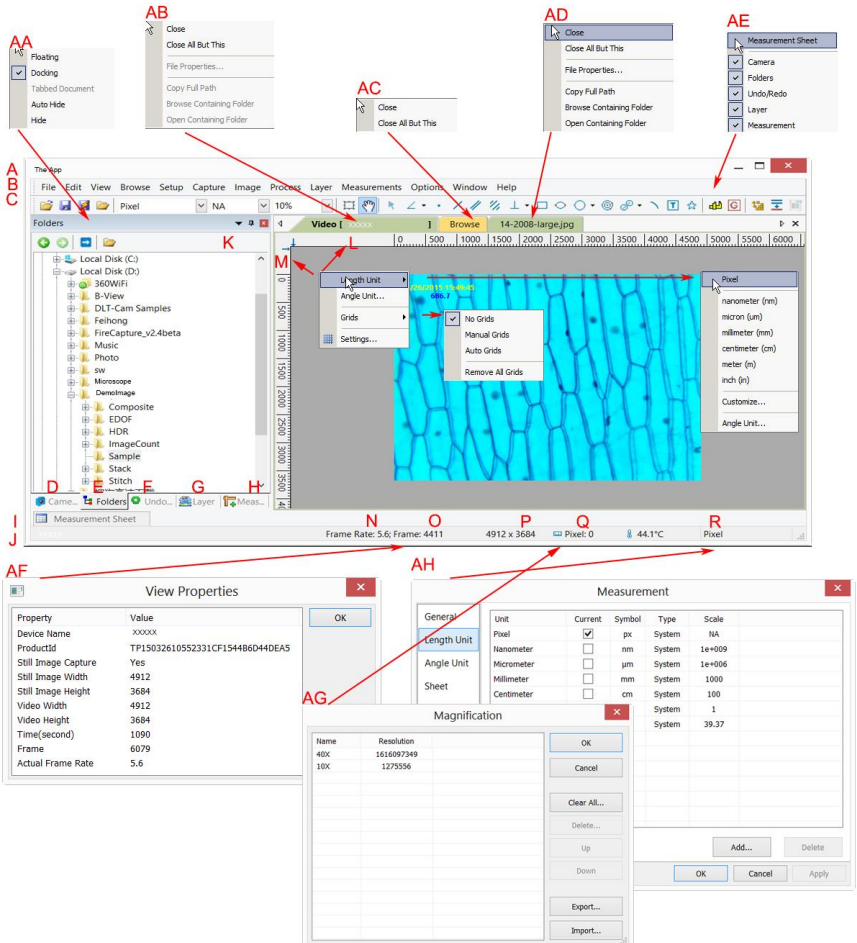

A: Image View;

B: Menu;

C: Image View toolbar

D: Camera Sidebar ;

E: Folders Sidebar ;

F: Undo/Redo Sidebar ;

G: [Layer Sidebar](#) ;

H: [Measurement Sidebar](#) ;

I: [Measurement Sheet](#);

J: [Statusbar](#);

K: [Auto Hide](#) button

L: [Horizontal ruler](#);

M: [Vertical ruler](#)

N: [Frame Rate](#)

O: [Frames](#) captured

P: Current [Video](#) sizes

Q: Selected microscope [Magnification](#)

R: Current [Unit](#);

AA: [Sidebar](#) right mouse button context menu;

AB: [Video](#) window right mouse button context menu;

AC: [Browse](#) window right mouse button context menu;

AD: [Image](#) window right mouse button context menu;

AE: [Frame](#) window right mouse button context menu;


AF: Double-click bring up [Video Properties](#) dialog;


AG: Double-click bring up [Magnification](#) dialog;

AH: Double-click bring up [Measurement](#) dialog;

AI: [Horizontal Ruler](#) or [Vertical Ruler](#) right mouse button context menu

### 2.2 How to close the video window?

1 Double-clicking the tabbed video window title or clicking **x** on  will close the video window directly;



2. Choose the [Windows>Close All](#) command to close the video window;


## Video Window GUI

---

3. Click the right mouse button on the video window title to invoke the context menu and choose [Close](#) to the video window.
4. Press [Ctrl+W](#).

### 3 Image window GUI

#### 3.1 Image window GUI

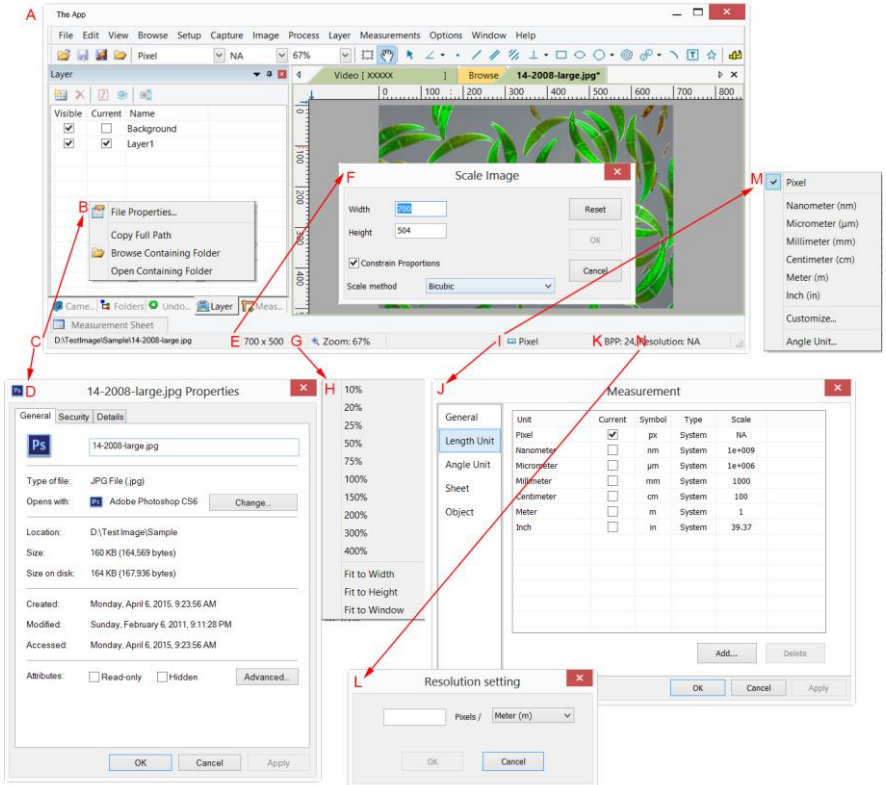

A: **ImageView**;

B: The opened file right mouse button context menu on status bar;

C: The opened file name and directory;

D: Double-click bring up opened file **Properties** dialog;

E: Current image width and height;

F: Double-click bring up **Scale Image** dialog;

G: Image **Zoom** ratio, double-clicking will zoom the image to 100%;

H: **Zoom** ratio right mouse button context menu;

I: Currently selected **Unit**;

J: Double-click bring up **Measurement** dialog;


K: Image **BPP** & **Resolution**;




L: Double-click bring up [Resolution Setting](#) dialog;


M: [Unit](#) right mouse button context menu.


### 3.2 How to close the image window?

1. If you have modified an image before attempting to close it, double-clicking the tabbed image window title or clicking [x](#) on  will bring up a [ImageView](#) dialog:

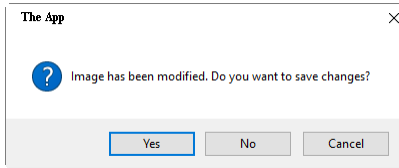

Clicking [Yes](#) will save the changes with its old name and close the window quickly, [No](#) will close the file immediately with no changes and no warning, or [Cancel](#) will cancel the [Close](#) command and leave the window there with no changes;

2. If the [Image](#) window is snapped from the video window and with number as its title, double-clicking the tabbed image window title or clicking [x](#) on  will bring up a warning [ImageView](#) dialog:

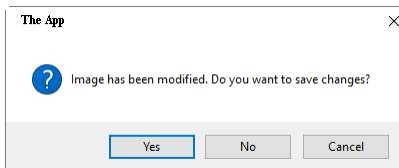


Clicking [Yes](#) will bring up the [Save As](#) dialog. In the [Save As](#) dialog, user can:

[Save in](#): Select the driver and folder to which you want your image file saved in the [Save in](#) combobox and enter the file name in the [File name](#) edit box;

[Save](#): Click [Save](#) to save the captured image with the specified directory and file name;

[Cancel](#): Click [Cancel](#) to close the [Save As](#) dialog and return to image window.

## Image window GUI

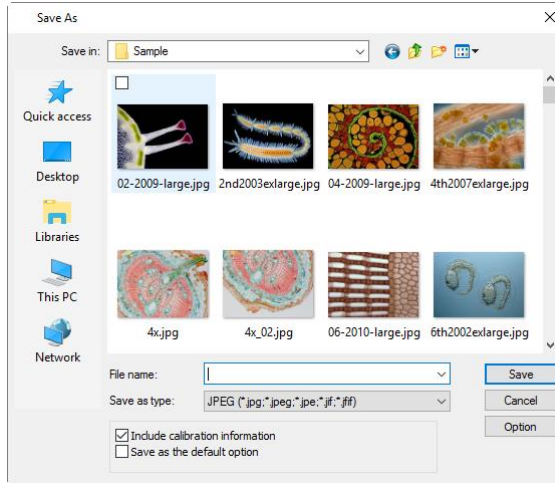

Click **No** on the **ImageView** dialog will close the file immediately with no changes and no warning

Click **Cancel** on the **ImageView** dialog will cancel the **Close** command and return to image window.

3. **Ctrl+W**;

**Note:** Choosing the **Window>Close All** command can also close the tabbed image window. Please check the **Window>Close All** for detail.

## 4 UI toolbar

When the camera is started or the image is opened (or captured), most of the icons on the toolbar will be available for the quick operation of the video or image window.




- 1: [Open](#) (Ctrl + O)
- 2: [Save](#) (Ctrl + S)
- 3: [Quick Save](#) (Quick Save)
- 4: [Browse](#) (Ctrl + B)
- 5: [Unit](#)
- 6: [Magnification](#)
- 7: [Zoom](#)
- 8: [Video/Image Select](#)
- 9: [Track](#)(enabled only when the video/image size is larger than the window size)
- 10: [Object Select](#)(will be enabled when an object is overlaid on the background layer)
- 11: [Angle](#)
- 12: [Point](#)
- 13: [Line](#)
- 14: [Parallel](#)
- 15: [Two Parallel](#)
- 16: [Vertical](#)
- 17: [Rectangle](#)
- 18: [Ellipse](#)
- 19: [Circle](#)
- 20: [Annulus](#)
- 21: [Two Circles](#)
- 22: [Arc](#)
- 23: [Text](#)
- 24: [Polygon](#)
- 25: [Scale Bar](#)
- 26: [Arrow](#)
- 27: [Calibrate](#) (for both video/image window)

- 28: [Gray Calibration](#) (for video window)
- 29: [Image Stitch](#)(for image or video window)
- 30: [Manual Fusion](#)(for image or video window)
- 31: [High Dynamic Range\(HDR\)](#)

## 5 Camera Sidebar

The **Camera Sidebar** is used for the control of camera, it includes many groups. The group can be expanded by a) clicking the group name or b) clicking the **Down Arrow** at the right end of the group name.



The down arrow to expanded the group

### 5.1 Camera List group

The 'Camera List' group is expanded, showing a list with one entry: 'XXXXX'.

**Camera List** will list all of the cameras connected to the computer that support the **ImageView** application. Click the camera name will start the camera video window.

### 5.2 Capture & Resolution group

The 'Capture & Resolution' group is expanded, showing 'Snap' and 'Record' buttons. Below are 'Live' and 'Snap' dropdown menus, both set to '2048 x 1534'.


**Snap**: Continuously **Snap** images by clicking it;  
**Record**: **Record** video stream in wmv/asf or avi format;  
**Live**: Set the video resolution;  
**Snap**: Set the **Snap** resolution for image capture.

### 5.3 Exposure & Gain group

The 'Exposure & Gain' group is expanded, showing 'Auto Exposure' checkbox, 'Exposure Target' slider (set to 120), 'Exposure Time' slider (set to 10.000ms), and 'Gain' slider (set to 1.00). A 'Defaults' button is at the bottom.

1. When the **Exposure & Gain** group is expanded, a green rectangle marked with "Exposure" will be overlaid on the video window. This marked region is a reference region for judging if the image brightness reach to the **Exposure Target** value. Drag or resize the **Exposure ROI** to the dark area will increase the video brightness and drag it to the brighter area will decrease the video

## Camera Sidebar



Rectangle for Auto Exposure

brightness;

2. Uncheck the [Auto Exposure](#) box to switch the [Auto Exposure](#) mode to the [Manual Exposure](#).


The [Exposure Target](#) slider will be disabled in this mode;

3. Tune the microscope light source to a bright state, and then drag the [Exposure Time](#) slider left or right until the image brightness is normal;

4. If and only if the microscope light intensity is too low to meet the [Exposure Time](#) up limit, drag the [Gain](#) slide right until the video brightness is normal;

5. The exact [Exposure Time](#) can also be entered by clicking the edit box at the right of the [Exposure Time](#). This will bring up a dialog called [Exposure Time](#). You can type the number in the field to set the exact [Exposure Time](#) value.

### 5.4 White Balance group

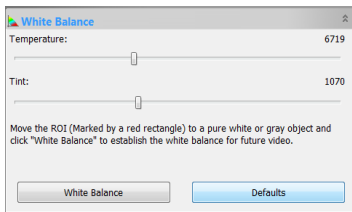

1. Click the [White Balance](#) bar to expand the [White Balance](#) group and a red rectangular marked with [White Balance](#) will be overlaid on the video window;


2. Drag or resize the red rectangle to a pure white or gray area and click the [White Balance](#) button to establish the video [White Balance](#) for future

video streaming process;

3. If the automatic setting and the actual result still has deviation, drag the [Temperature](#) and [Tint](#) slides to left or right to manually correct the [White Balance](#).


### 5.5 Color Adjustment group

## Camera Sidebar

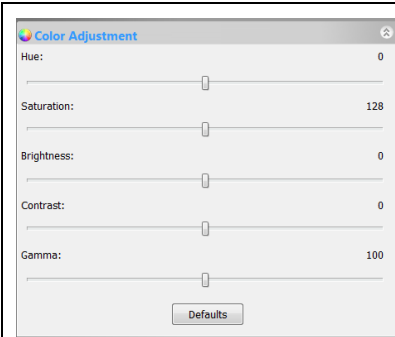


1. **Hue**: Adjusts the **Hue** of the video. Drag the slider to the right to increase or drag to the left to decrease **Hue**;
2. **Saturation**: Adjusts the **Saturation** of the video. Drag the slider to the right to increase or drag to the left to decrease video **Saturation**;
3. **Brightness**: Adjusts the video **Brightness**. Drag the slider to the right to increase or drag to the left to decrease the video **Brightness**;
4. **Contrast**: Adjusts the video **Contrast**. Drag the slider to the right to increase or drag to the left to decrease the video **Contrast**;
5. **Gamma**: Adjusts the video **Gamma**. Drag the slider to the right to increase or drag to the left to decrease the video **Gamma**;
6. **Defaults**: Click the **Defaults** to clear all the changes and reset them to default ones;
7. All of your settings will be saved for future **Color Adjustment** group.

### 5.6 Frame Rate group

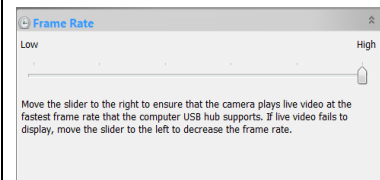


- Drag the slider to the right (**High**) to ensure that the camera can run the video at the fastest **Frame Rate** that the computer USB hub supports. If the video fails to display, drag the slider to the left (**Low**) to reduce the **Frame Rate** and this will enable the video to stream in a low speed mode.

### 5.7 Flip group



- If the video on the screen appears in different directions from what is viewed under the camera, check the "**Horizontal**" or "**Vertical**" box to set the video direction to the right one.


### 5.8 Color/Gray group



- If you wish to preview **Color** video, select the "**Color**" button, otherwise, check the **Gray** button.
- If you wish to preview **Gray** video, check the "**Gray**" button.

### 5.9 Power Frequency group

## Camera Sidebar



1. A CMOS sensor captures each row of pixels (from top to bottom) in sequential order, creating a rolling effect, hence the name "Rolling Shutter". Instead of being relatively constant, so for example, as the commercial main frequency in Europe is 50Hz, fluorescent lights in Europe flicker at 100 times per second and as the main frequency in US is 60Hz, so in the USA they flicker at 120 times per second;
2. This flickering problem is solved by capture row pixels in over the duration of integer number of (n) flicker periods;
3. check **50HZ** will delete the rolling dark band for the **50HZ** light fluctuation;
4. check **60HZ** will delete the rolling dark band for the **60HZ** light fluctuation;
5. For **DC** power, no light fluctuation is existed and no compensation is needed.

### 5.10 Sampling group



1. **Bin**: Pixel binning refers to the method of combining (averaging) pixels of blocks of neighboring same color pixels to resize the video to the lower resolution;
2. **Skip**: Also called "Decimation", means that a certain amount of pixels are not read out but skipped (horizontally, vertically or in both axes). This reduces resolution of the resulting video but introduces subsampling artifacts.

### 5.11 Bit Depth group



Switch between **8 bits** and **12 bits**. **8 bits** is the basic Windows image format. **12bits** will have higher image quality but moderate FPS.

### 5.12 ROI group




**ROI**, Region of interest. This function can set the **ROI** on the video window. When the **ROI** group was expanded, a dotted rectangle with "Handles" will appear around the video window that will let you alter the **ROI**. Use mouse button to adjust the **ROI** size. If **ROI** is ok, click **Apply** will set the video to **ROI** size, **Defaults** will return to the original size.

### 5.13 Histogram group




## Camera Sidebar

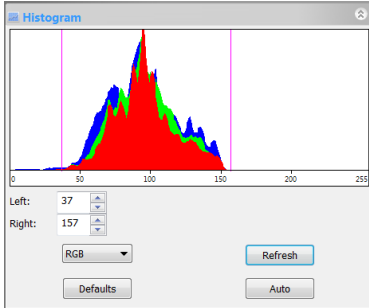

1. A **Histogram** illustrates how pixels in an image are distributed by graphing the number of pixels at each color intensity level. The **Histogram** shows detail in the shadows (shown in the left part of the histogram), midtones (shown in the middle), and highlights (shown in the right part). A **Histogram** can help you determine whether an image has enough detail to make a good correction;
2. This group shows the **Histogram** of current active video. Two vertical line markers show the upper and lower limits of the intensity levels. These markers can be dragged with mouse. If you are looking at a color image, the **Histogram** will reflect the **RGB**(red, green and blue channels histogram at the same time) **R**(red), **G**(green), and **B**(blue) values with lines of the same color;
3. You can also enter directly the desired values in the **Left** or **Right** boxes below the **Histogram** chart for both **Left** and **Right Histogram** boundaries;
4. Click the “**Refresh**” button to update the **Histogram** display if the sample under observation is moved or changed;
5. Clicking the **Defaults** button will return the **Left** and **Right Histogram** boundaries to its original ones;
6. Click the **Auto** button to locate the two boundaries automatically to get the best video quality.


### 5.14 Dark Field Correction

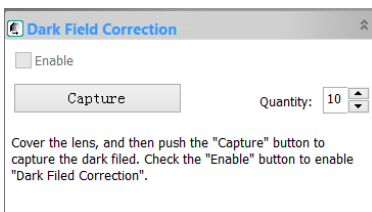

To **Enable** the **Dark Field Correction**, one should capture the dark field image first. After the images are captured, the **Enable** button will be enabled. Check it will enable the **Dark Field correction**. Uncheck is will disable the **Dark Field Correction**.


### 5.15 Misc

## Camera Sidebar

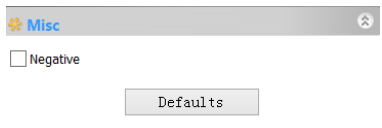

**Negative** will reverse the pixel values of the active video without going through the lookup table.

### 5.16 Parameters group



**Parameters** group is used to save the camera control parameters adjusted for further application.

Click **Save** will save the current camera control parameters with new parameter file; The **Load** and **Overwrite** buttons will be enabled.

Click **Load** will load the saved camera control parameters;

Click **Overwrite** will overwrite the current camera control parameters to the current loaded active camera control parameters file;

Click **Management** will invoke a **Management** dialog and in this dialog, one can manage all of the saved **Parameter** files.


## 6 File

### 6.1 Open Image(O)●●●

**Ctrl+O**

Choose the **File>Open Image●●●** command to open an existing image file. The **Open Image●●●** command can also be used to preview an image in small size, or to view its statistics and information without actually opening the image itself. These capabilities can be used to quickly locate a particular image.

**ImageView** supports and can open many image formats. These are identified in the **Files of type** list box. You may also open an image file type with **ImageView File Type (\*.tft)** format which can save **Measurement Objects** (for simplicity, only **Object** or **Objects** will be used to represent **Measurement Object** or **Measurement Objects**) overlaid on the image.

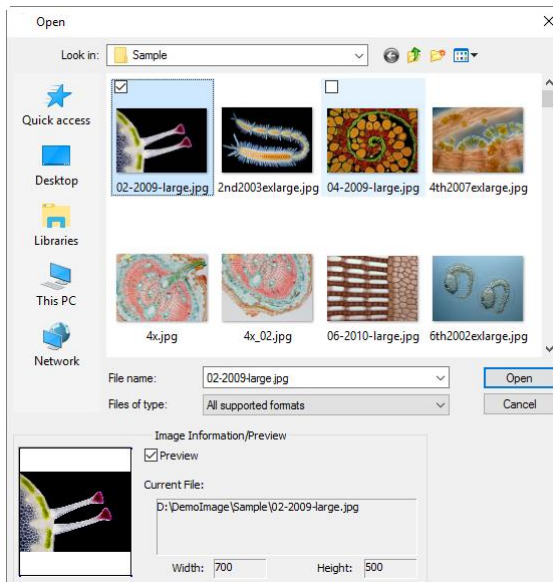

More than one image can be opened within **ImageView** simultaneously by a) with **Ctrl + left mouse button** method and b) **Shift + left mouse button** method to highlight the files to be opened. In this mode, the **Preview** window will be disabled.

When opening an image, **ImageView** places it into a new image window. It then becomes the active image.

**Note:** [ImageView](#) maintains, at the [File>Recent Files](#) submenus, a list of the last 4 (Can be 1-8) opened files. Any of these files can be accessed by simply clicking on file name. If no files are listed in the [File>Recent Files](#) submenu, the [Open Image...](#) command must be used to open the file.

Also, the [View>Browse](#) can be used to view images in an [Icon](#) format under any selected directory. Brief information is given in the [View>Browse](#) menu.

**File name:** From this list box, select the name of the file want to open. Either the type of the file name (with its entire path, if it is not in the current folder), or selecting [Files of type](#) to obtain a list of file names. Double-clicking a file name in the large combo box (where both folder and file names are listed) will automatically open it.

**Note:** If just type in the file name, be sure that the [Files of type](#) field correctly identify the format of the file to open. Otherwise error messages will bring up when [ImageView](#) tries to open the file.

**Files of type:** In this list box, select the image format of the file to open. If one selects [All supported formats](#), [ImageView](#) uses the file's extension to identify its format.

[ImageView](#) supports the following file formats:

Window Bitmap(\*.bmp,\*.dib,\*.rle)

JPEG(\*.jpg,\*.jpeg,\*.jpe,\*.jif,\*.jfif)

Portable Network Graphics(\*.png)

Tag Image File Format(\*.tif, \*.tiff)

CompuServe GIF (\*.gif)

PCX(\*.pcx)

Targa(\*.tga)

PhotoShop(\*.psd)

Icon(\*.ico)

Enhanced Window Metafile(\*.emf)

Window Metafile(\*.wmf)

JBIG(\*.jbg)


Wireless Bitmap(\*.wbmp)

JPEG 2000 Standard(\*.jp2)

JPEG 2000 Codestream(\*.j2k)

Digital Imaging and Communication in Medicine(\*.dcm)

Digital Negative(\*.dng)

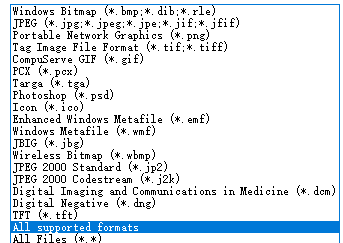

### ImageView File Type(\*.tft)

If the image file does not use standard format-identifying extensions, the file in the **File name** field must be typed, and then select its format from the **Files of type** list box. Otherwise, **ImageView** will select a format based on the file name extension.

**Preview:** Click this button to preview image in small size. In preview mode, statistics and information about the image (i.e. image **Width**, **Height** and image location) will be displayed. The default is no **Preview**.

**Current File:** **Current File** location on your computer;

**Width:** **Current File** image width;


**Height:** **Current File** image height;

### 6.2 Open Video(V)●●●



The **File>Open Video●●●** menu will be enabled only when there is no video file opened in the **ImageView** frame or no camera was opened.

1. Choose the **File>Open Video●●●** command to open an existing video file;

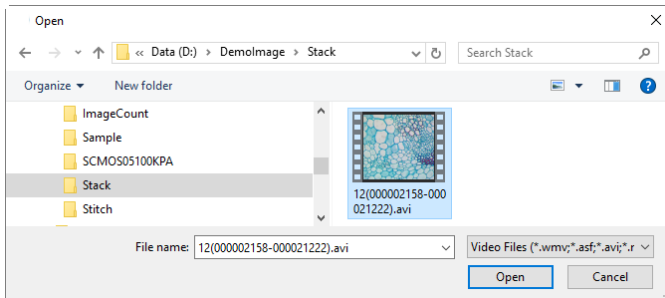

2. Select the name of the file you want to open. If the file does not appear, select the option for showing all files from the **Files of Type** combobox. The video file type can be **\*.wmv\***, **\*.asf\*** or **\*.avi\*** format.

3. Click **Open** to open a video file, this will create a video window and begin to start the video stream. The video window will be associated a name called "**Video [XXX.XXX]**" (i.e., its title bar will display "**Video [XXX.XXX]**", here, **XXX.XXX** is the video file name).


4. Click **Cancel** to return to the application.

**Note:** Only a single video can be opened at a time. **ImageView** takes camera as a

special video file, if the camera was opened, this menu will be disabled and the video file cannot be opened anymore.

### 6.3 Open Broadcast(C)●●●

Users could receive the broadcasting video by [ImageView](#) from the other user by the [Address](#) and [Port](#). For example, if a user starts a broadcasting service via [Address](#) 192.168.0.20 and [Port](#) 2080, the other users could share the video that is opened on 192.168.0.20 by inputting the right [Address](#) and [Port](#). If the receiver and the broadcaster are in one intranet, the performance will be excellent. If not, the performance will depend on the bandwidth.

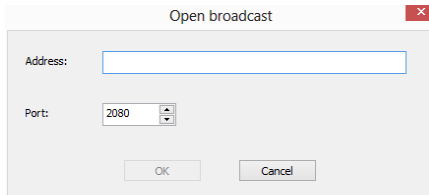

### 6.4 Save(S)



**Ctrl+S**

Choose the [File>Save](#) command to immediately store the current window image to its file (the file name is listed on the window's title bar) while leaving the image still active in its window.


If the image is untitled or titled with a digit, [ImageView](#) will issue the [File>Save As●●●](#) dialog automatically. The default "Save as type" will be "Window Bitmap (\*.bmp,\*.dib,\*.rle)". If there are [Objects](#) overlaid on the image, the default [Save as type](#) will be "ImageView File Type (\*.tft)".

The [File>Save](#) command can be used to save the most recent changes to disk. It is often performed as a precautionary measure during lengthy or involved processes to reduce the amount of reprocessing that might be required in the event of a system failure or operational error. When an image is closed and not to save its changes is chosen, [ImageView](#) discards all changes made since the last [File>Save](#) operation.

**Note:** a).The [File>Save](#) command always saves the contents of the entire window, even if there is an [AOI \(Area of Interest\)](#) defined on it; b).The [File>Save](#) command will be disabled if the file is not changed or the changes have been saved.

## 6.5 Save As(A)●●●

Choose the **File>Save As●●●** command to store the contents of the current window to a specified file format. At the end of a **File>Save As●●●** operation, the image window will be associated with the new file and the new format (i.e., its title bar will display the new file name).

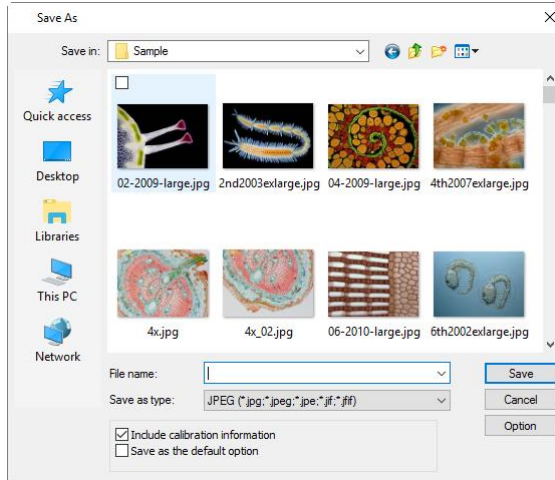

ImageView supported file save formats are:

- Window Bitmap(\*.bmp,\*.dib,\*.rle)
- JPEG(\*.jpg,\*.jpeg,\*.jpe,\*.jif,\*.jfif)
- Portable Network Graphics(\*.png)
- Tag Image File Format(\*.tif, \*.tiff)
- Compuserve GIF (\*.gif)
- PCX(\*.pcx)
- Targa(\*.tga)
- JBIG(\*.jbg)
- JPEG 2000 Standard(\*.jp2)
- JPEG 2000 Codestream(\*.j2k)
- Digital Imaging and Communication in Medicine(\*.dcm)
- ImageView File Type(\*.tft)

**Save in:** Find the folder where the file wishes to be saved. A new folder may be

created using the [New Folders](#) button;

**File name:** The file name to be saved. To specify the file's location, either enter its entire path (disk and folder), or specify its location using the [Save in](#) list box;

**Save as type:** In this list box, select the format in which the image wants to be saved.


**Save As...** is also used to convert a single image from one format to another. For example, if a [TIFF](#) file needs to convert to [PCX](#) format, open the [TIFF](#) image first, then choose [Save As...](#) command with the [PCX](#) format to save it to a new file.

The default "Save as type" will be "Window Bitmap (\*.bmp,\*.dib,\*.rle)". If there are [Objects](#) overlaid on the image, the default [Save as type](#) will be "ImageView File Type (\*.tft)".

The [Save As](#) command has several important uses beyond simply storing an image to a new file name. Click [Option](#) to select the different parameters to encode the file.

### 6.5.1 Option for JPEG

For [JPEG](#) (\*.jpg,\*.jpeg,\*.jpe,\*.jif,\*.jfif), [Option](#) has the following items:

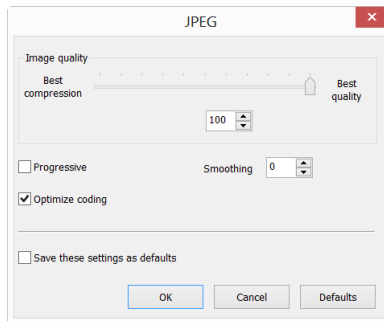

**Image quality:** If one save an image in [JPEG](#) format (\*.jpg), one may adjust image quality in the edit box. The values range from 0 to 100. Default value: 75;

**Progressive:** The default is unchecked;

**Optimize Huffman codes:** The default is unchecked;

**Smoothing:** The values range between 0 and 100. Default value: 0;

**Save these setting as defaults:** When saving a file, the current settings will be saved




as defaults for the next file save operation.

### 6.5.2 Option for PNG

For [Portable Network Graphics \(\\*.png\)](#), [Option](#) has the following items:


[Interlaced](#): The default is unchecked;

[Save these setting as defaults](#): When saving a file, the current settings will be saved as defaults for the next file save operation.

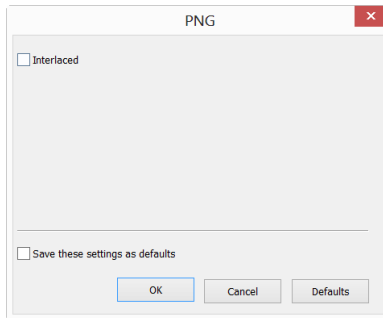

### 6.5.3 Option for TIF

For [Tag Image File Format \(\\*.tif, \\*.tiff\)](#), the [Option](#) has the following items:

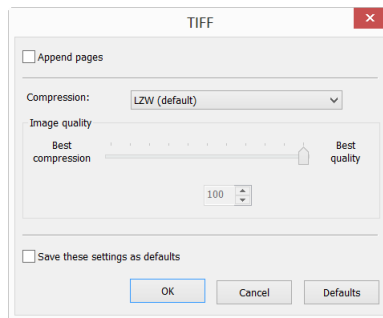

[Appended pages](#): Determine whether the current image will be saved in multiple pages style or not;

[Compressions](#): Specifies a method for compressing the composite image data. For saving a 32-bit [TIFF](#) file, one can specify that the file be saved with predictor compression, but have no option to use [JPEG](#) compression. Predictor compression


offers improved compression by rearranging floating point values, and works with both [LZW](#) and [ZIP](#) compression;

**Image quality:** If choosing [Compressions](#) as "JPEG", the [Image quality](#) can be adjusted by the slider bar. The values range between 0 and 100. Default value: 75;

**Save these setting as defaults:** When saving a file, the current settings will be saved as defaults for the next file save operation.

#### 6.5.4 Option for JPEG 2000 Stanndard, JPEG 2000 Codestream

For [JPEG 2000 Standard](#), [JPEG 2000 Codestream](#), Option has the following items:

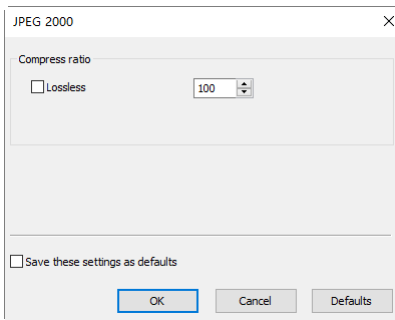

**Lossless:** Can check the [Lossless](#) or its right edit box with spin button to choose the wished compress ratio. The default value is 100(1~100);


**Save these settings as defaults:** Save the current settings as defaults and application and need not to reset is again in future application;

#### 6.5.5 Option for Digital Imaging and Communication in Medicine(\*.dcm)

For [Digital Imaging and Communication in Medicine](#), Option has the following items:

**Compression:** There are 3 terms in the drop down box, they are [Lossless JPEG](#)(default), [RLE](#), [None](#). The default is [Lossless JPEG](#);


**Save these settings as defaults:** Save the current settings as defaults and application and need not to reset is again in future application;

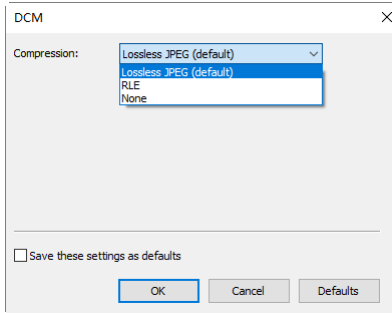

### 6.5.6 Option for the other formats


For [Compuserve GIF \(\\*.gif\)](#); [PCX\(\\*.pcx\)](#); [Targa\(\\*.tga\)](#); [JBIG\(\\*.jbg\)](#); [ImageView File Type\(\\*.tft\)](#), There is no [Option](#).

**Note:** a) Detailed information of the above academic terminologies can be found in books about image processing and image compression or internet; b) The file saved directory can be restored for future use. To keep the directory unchanged when [ImageView](#) is started again, choose [Options>Preferences...](#) command, click [Misc](#) page and check [Restore the current directory when startup](#) under the [Privacy](#) item.

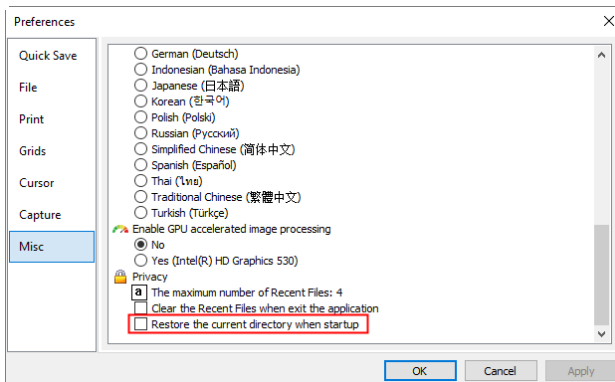

### 6.6 Batch Save(B)...

The [File>Batch Save...](#) menu will be enabled when a) an image is opened; b)an image is captured from the camera; c)an image window is created by choosing the [File>Paste as New File](#) command; d)an image window is copied from the [Undo/Redo Sidebar](#) with the copy button as show below:



Current	Index	Operation
<input checked="" type="checkbox"/>	1	Open

## 6.6.1 Batch Save for a) style image window


1. If the image is modified, choosing the [File>Batch Save...](#) command will save the file with its opened file name and file extension;
2. If the image is modified because of the [Objects](#), choosing the [File>Batch Save...](#) menu will save the file with its opened file name but with "ImageView File Type (\*.tft)" file extension format;

## 6.6.2 Batch Save for b), c) or d) style image window

If the image window has been created with b), c) or d) style, choosing the [File>Save As...](#) command to realize the file saving task will be time-consuming. The [Batch Save...](#) command will runs [File>Save As...](#) command with the name automatically specified according to the paradigm specified in the [Batch Save](#) dialog

To start the [File>Batch Save...](#) command for b) style image window, you have to

1. Start the camera;
2. Snap at least an image first;
3. Choosing the [File>Batch Save...](#) command will bring up a [Batch Save](#) dialog:

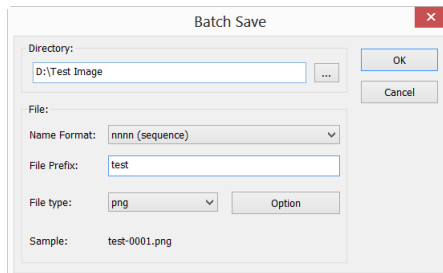

**Directory:** Enter the name of the drive and directory where your captured images will be saved. You may either type the path information, or use the [Browse](#) button to locate it from a standard [Browse Folder](#) dialog.

**Name Format:** The [year](#), [month](#), [date](#), [hour](#), [minute](#) and [second](#) or [nnnn\(sequence\)](#) are used to as part of the file name. If more files are saved with in a second, a [\(xx\)](#)

suffix is attached to the end of [Name Format](#) to avoid the possible name conflict. For the [nnnn\(sequence\)](#) "[Name Format](#)", no suffix is needed.

**File Prefix:** Enter a file name prefix for [Batch Save](#) when generating files names for a series of images. This prefix will be combined with [Name Format](#) to form a final file name naming paradigm.

**File Type:** In this combobox, select the format in which you want the image to be saved (can be [BMP](#), [JPG](#), [PNG](#), [TIF](#)). Click [Option](#) button to set the different parameters for encoding the file (For [BMP format](#), the [Option](#) will be disabled. See [File>Save As...](#) menu about the details of the format encoding methods); If there are [Objects](#) over the image, the [File Type](#) will be chose as "[ImageView File Type \(\\*.tft\)](#)" by [ImageView](#).

**Sample:** The final file name is shown at the right of the [Sample](#) label for reference.

4. If the setting in the [Batch Save](#) dialog was finished, click [OK](#) button to begin the file batch save process or [Cancel](#) to cancel the [Batch Save](#) command and return to the application.

For the c) or d) style image window, only steps 3 and 4 are needed.

**Note:** a) In the process of the [File>Batch Save...](#) command, the title on the image tab or image window will be modified with the file name paradigm in the [Batch Save](#) dialog. b) The [File>Batch Save...](#) will perform no saving operation if the file is not modified or unchanged.

### 6.7 Quick Save(Q)




### CTRL+Q

The [File>Quick Save](#) menu will be enabled when a) a new image captured from the camera; b) an image window is created by choosing the [File>Paste as New File](#) menu; d) an image window is copied from the [Undo/Redo Sidebar](#) with the copy button as show below:

Current	Index	Operation
<input checked="" type="checkbox"/>	1	Open

[File>Quick Save](#) can save the file at quick way with no need to specify the file directory, file name and file format. All those are specified in [Options>Preferences...](#), [Quick Save](#) property page. The file name can be renamed according to the setup in

the [Options>Preferences](#)..., [Quick Save](#) property page's [Show the rename dialog](#) item.

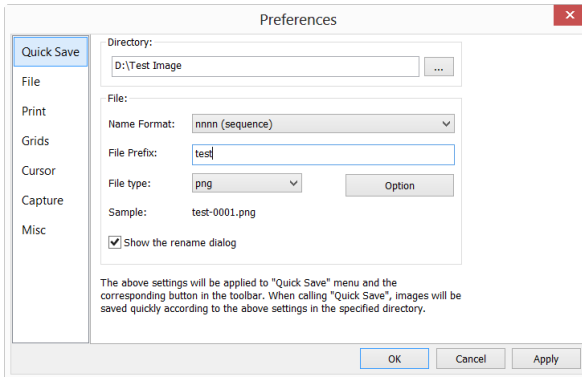

## 6.8 Paste as New File(N)

The [File>Paste as New File](#) menu will be enabled only when there is valid image data on the clipboard first (see the [Edit>Copy](#) menu). If there is no image data on the clipboard, the [File>Paste as New File](#) menu will be disabled.

Choose the [File>Paste as New File](#) command to place the contents of the clipboard image into a new image window, which becomes the active image.

The new image type will be the same as that of the original image. [ImageView](#) will accept image data from other applications via the clipboard as long as it is in [Windows Bitmap \(DIB\)](#) format.

**Note:** [ImageView](#) will assign a digit to the [Paste as New File](#) command created image window title bar.

## 6.9 Twain: Select Device


[Twain](#) is a cross-platform interface for acquiring images captured by certain scanners, digital cameras, or frame grabbers. The manufacturer of the [Twain Device](#) must provide a [Source Manager](#) and [Twain Data Source](#) to work with [ImageView](#).

Select the active device for the [Twain: Acquire](#) menu from all devices available in the device combobox which are enumerated by the application.

One must install the [Twain Device](#) hardware and its driver first. See the

documentations provided by the device manufacturer for the installation instructions.

Before begin to start the **Twain: Acquire** at the 1st time with **ImageView**, choose the **File>Twain: Select Device...** command first, this will invoke a dialog called **Select Source** as shown below:

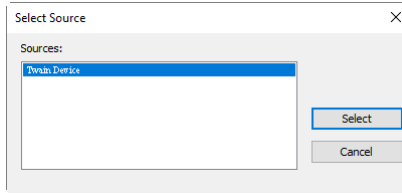

**Source:** Choose the right device from the **Source** window (Highlight it)

**Select:** Click **Select** to select the device. User does not need to repeat this step for subsequent choosing of the **Twain: Acquire...** command.

**Note:** All of the **ImageView** cameras are integrated into one **Source** called **Twain Camera**. This will greatly reduce the list item and easy to choose for the user.

## 6.10 Twain: Acquire...

### 6.10.1 Introduction

There are basically two techniques used to capture the video images from video devices such as a PC camera, digital camera, and scanner. They are the **Twain: Acquire...** technique and the **DirectShow** technique (previously called **VFW**).


The most obvious characteristics of the **Twain** technique is that it previews the video in smaller resolution but captures the image with higher resolution. The **ImageView** series cameras support all of these two video preview techniques.

### 6.10.2 Steps for Twain Acquire

Here we illustrate how to capture the image using a **XXXXX** (3.1M pixels, USB3.0) camera as an example.

1. Install the camera **Twain** driver provide by the supplier (for example driver for **XXXXX** hardware);
2. Install **ImageView**;

3. Plug the cameras **XXXXX** (USB3.0) into the computer;
4. Start **ImageView**;
5. Choose the **File>Twain: Select Device...** command to select the device from the **Select Source** dialog (If never selected before);
6. Choose the **File>Twain: Acquire...** command. There should be a dialog box like below:

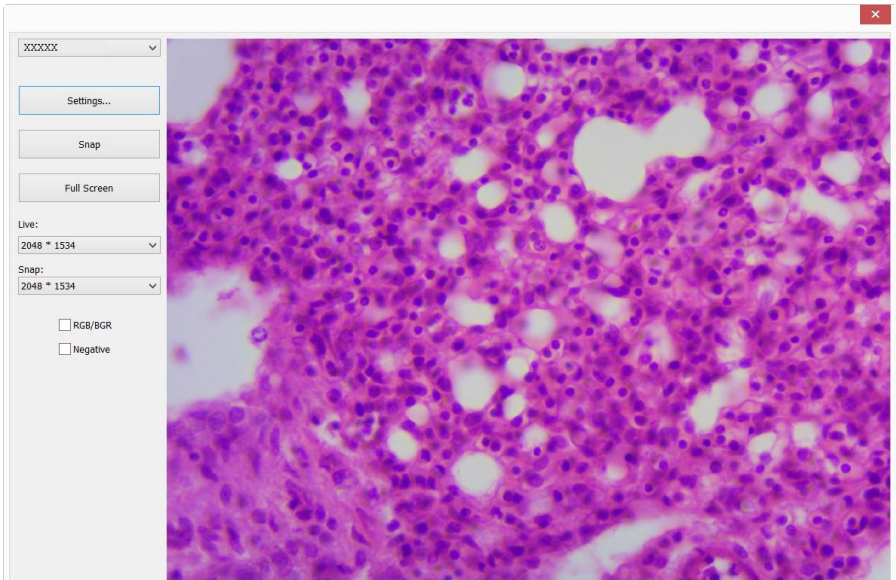

In this dialog, the video **Resolution** can be chosen. The **Video Source Property** can be set by clicking the **Setting...** button. Click the **Snap** button to capture an image. This will create a new window and its title bar will be assigned a digital as the image window name;

Check the **RGB/BGR** box to ensure the correct color encoding format compatible with your application.

Click **X** on the window's upright corner to close the **Twain: Acquire** dialog.

### **6.11 Print Setup(R)...**



Choose the [File>Print Setup...](#) command to access the setup panel for the printer that has selected. [ImageView](#) will present the standard setup panel for the particular printer (this is the same panel one would receive if one were setting up the printer from the [Windows Control Panel](#)). Change printer's setup to satisfy the requirements, click [OK](#) button to return.

### 6.12 Print Preview(V)... Ctrl+Shift+P

Choose the [Print Preview](#) command to see the real-time effect of the printer without actually printing it out.

### 6.13 Print(P)...



**Ctrl+P**

Choose the [File>Print...](#) command to print one or more copies of the current image to the selected output device. The [ImageView File>Print...](#) command lets one take full advantage of the printer's capabilities. If the printer has built-in half-toning or color dithering capabilities, use them or instruct [ImageView](#) to perform these processes before sending the image to the device.


The [File>Print...](#) command also has facilities that let one adjust the size and position of the image on the printed page.

### 6.14 Recent Files

[ImageView](#) maintains 4 (default) most recently opened document files under the [Recent Files](#) menu. Choosing one of these submenus will reopen that file immediately.

**Note.** a) The [maximum number of Recent Files](#) can be modified by choosing the [Options>Preferences...](#) command and clicking the [Misc](#) page as shown below:


Here, clicking the 4 (default) edit box will allow you to enter the number of the [Recent Files](#) submenus that you want. The value ranges from 0 to 8, the default is 4; b) One can also check the [Clear the Recent Files when exit the application](#) to clear the [Recent Files](#) after exit [ImageView](#) application.

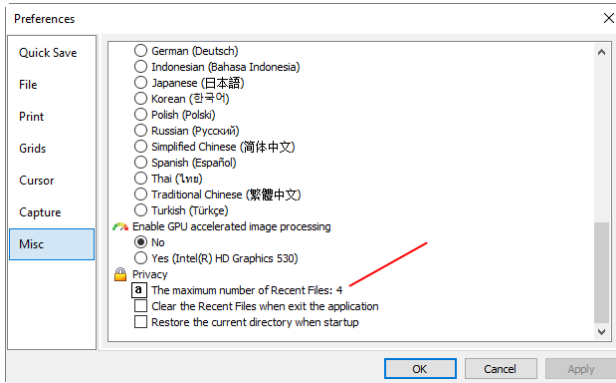


### 6.15 Exit(X)

Choosing the **File>Exit** command will close video, all of the image windows and **Browse** window. After all of the windows are closed, **ImageView** will end itself.

**Note:** If an image has been modified before attempting to **Exit** it, **ImageView** will issue a warning to ask if user want to save the image or not first.

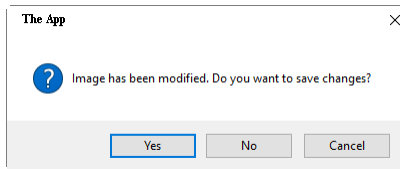

If multiple images have been modified before attempting to **Exit** it, **ImageView** will issue **Save Files** dialog to direct the user to save changes in different ways.

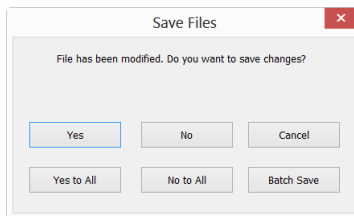

See **Window>Close All** for details.

## 7 Edit

### 7.1 Cut(T)



**Ctrl+X**

The **Edit>Cut** menu will be enabled only when a) an **Object** or **Objects** on the **Layer** over the image is or are selected; b) an image or images in the **Browse** window is or are selected.

#### 7.1.1 Cut for Objects

Check the **Measurements>Object Select**  or **Edit>Select All** menu to find how to select **Layer Objects** for the **Edit>Cut** command.

Choose the **Edit>Cut** command to a) copy the selected **Objects** to the clipboard and b) delete the selected **Objects** on the image. Any data already exist on the clipboard will be replaced.

The **Objects** copied to the clipboard can be pasted into the active window or into another opened video/image window on the layer overlaid on the image using the **Edit>Paste** command (when there is no **Layer** overlaid on the **Background**, **ImageView** will create a new **Layer** first).

#### 7.1.2 Cut for Browse window selected files

When the **Browse** window is active and the image files in the **Browse** window are selected, the **Edit>Cut** command will be enabled. Choosing the **Edit>Cut** command will delete the selected files and copy it to the clipboard.

**Note:** The **Edit>Cut** command does not support **Background Layer** (image) **Cut** operation.

### 7.2 Copy(C)




**Ctrl+C**





Choose the **Edit>Copy** command to **Copy** the highlighted **Objects** (on **Measurement Layer**) or an image's selected area on the **Background Layer** to the clipboard.


Note: When a) the **Object(s)** is (are) highlighted or b) the **Current Layer** is the **Background Layer** and an image ROI is selected, the **Edit>Copy** menu will be enabled.

### 7.2.1 Copy the selected area on the background layer to the clipboard.

1. Select the image area using the **Image Select**  button on the toolbar. The **Edit>Copy** menu will be enabled;
2. Choose the **Edit>Copy** command to copy the selected image area to the clipboard.

### 7.2.2 Copy object(s) on the measurement layer to the clipboard.

1. For the **Layer** operation, see the **View>Sidebar>Layer** menu in Sec.8 and the **Layer** menu in Sec.14 for details;
2. For the **Measurement** operation, see the **View>Sidebar>Measurement** menu in Sec.8 and the **Measurements** menu in Sec.15;
3. After the **Measurement** operating has been done, choose **Measurements>Object Select** command or check the **Object Select** button , the cursor will change to  in the video/image window;
4. Move the mouse until the cursor becomes , this means the cursor is right on the **Object**. Clicking it will highlight **Object** and select the **Object**;
5. Option 1: Continue to move the mouse until the cursor becomes  again, this means the cursor is right on another **Object** again. Clicking it with **Shift+left mouse button** and the second **Object** will be selected and highlighted;
6. Option 2: a) Move the cursor over the image, click down the left mouse button; b) Drag the mouse to draw a rectangle on the image. A dotted rectangle will appear around the selected area; c) Release the mouse and all of the **Objects** within the dotted rectangle will be highlighted and selected;
7. After the **Objects** are selected, the **Edit>Copy** menu will be enabled;

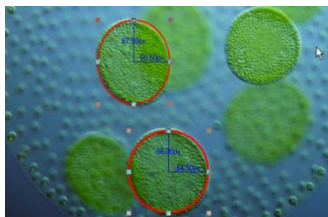

8. Choose the **Edit>Copy** to **Copy** the **Object(s)** to the clipboard. Then the **Edit>Paste**

menu will be enabled. One can then **Paste** the objects onto the **Current Layer** or onto the other **Measurement Layer** in the same video/image window. If one switches to the **Background Layer**, the **Edit>Paste** menu will be disabled, but if one returns to the **Measurement Layer** again, the **Edit>Paste** menu will be enabled again.

### 7.2.3 Copy for Browse window selected files

When the **Browse** window is active and the image files in the browse window are selected, the **Edit>Copy** command will be enabled. Choosing the **Edit>Copy** command will copy the image files to the clipboard. After the **Edit>Copy** command, the **Edit>Paste** and the **Edit>Paste** shortcut menus will be enabled.

**Note:** a) The **Edit>Copy** command will not delete the **Objects** over the image. Any data existing on the clipboard will be replaced with the new data; b) The copied **Object(s)** can be pasted into the active window or into another opened window using the **Edit>Paste** command as long as the current window is not on the **Background Layer** (the **Edit>Paste** menu will be disabled if the **Background Layer** is active). See the **View>Sidebar>Layer** command in Sec.8 and the **Layer** menu in Sec.14 for details; c) the copied files on the clipboard can be pasted into the Browse window by choosing the **Edit>Paste** command.

### 7.3 Paste(P)



**Ctrl+V**

If a) there is (are) **Object(s)** on the clipboard and the **Current Layer** is not the **Background Layer**, or b) there is (are) image file(s) on the clipboard and the current active window is Browse window, the **Edit>Paste** menu will be enabled.

#### 7.3.1 Paste for Objects

Choose the **Edit>Paste** command to **Paste Objects** from the clipboard onto the active image's **Measurement Layer**. One can also choose **Edit>Paste** command to transfer a layer's **Objects** from one image window's **Measurement Layer** to another image window's **Measurement Layer**.


#### 7.3.2 Paste for Browse window selected files

When the **Browse** window is active and the image files in the browse window are selected, the **Edit>Paste** command will be enabled. Choosing the **Edit>Paste** command will paste the clipboard files to the **Browse** window.

**Note:** The **Edit>Paste** command does not support the image area **Paste** operation.

## 7.4 Paste Shortcut(S)

This command is for [Browse](#) window only. This menu will be enabled when files in the [Browse](#) window are selected and the [Edit>Copy](#) command is executed to copy the file shortcut to the clipboard. Choose this command will create the selected files [Shortcut](#)(in \*.lnk format) in the current [Browse](#) window.

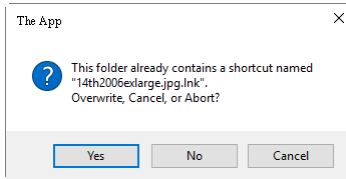

If the to be pasted \*.lnk file has been existed in the current [Browse](#) window, [ImageView](#) will pop up a prompt dialog.

One can click [Yes](#), [No](#) or [Cancel](#) to [Overwrite](#), [Cancel](#) or [Abort](#) the command.

## 7.5 Delete(D)



## Delete

The [Browse>Delete File](#) menu will be enabled if a) the file(s) is (are) highlighted in the [Browse](#) window, b) the Object(s) on the video/image are selected. This command is for [Browse/Video/Image](#) window only.

You can [Delete](#) or remove one or more files from the [Browse](#) window. The steps are as follows:

### 7.5.1 For Browse Window file delete

1. Select one or more files by a) Clicking the displayed file icons, a single file will be highlighted; b) Clicking the file one by one with [Ctrl + left mouse button](#), all of the clicked files will be highlighted; c) Clicking the displayed file icons, the first clicked file will be highlighted, clicking the end file with [Shift + left mouse button](#), all of the files among the first and last will be highlighted. d) Dragging the mouse to draw a dotted line rectangle across the files you wish to delete, all of the files in the rectangle will be highlighted; e) [Ctrl+A](#) to select whole files in the [Browse](#) window
2. a) Press the [Delete](#) key to delete the selected files; b) Click your right mouse button to bring up a context menu, choose the [Delete](#) command to delete the highlighted files. A [Confirm File Delete](#) dialog will bring up.



In the **Confirm File Delete** dialog, click **Yes** to move the files to the desktop recycle bin, or **No** to cancel the **Delete** operation.


### 7.5.2 For Video/Image Window Object delete


If the **Objects** on the video/image are selected, choosing **Browse>Delete** File or pressing delete button will remove the **Object** from the video/image window.

### 7.6 Image Select(S)

The **Edit>Image Select** command can be used to mark **ROI** and **Copy** the selected **ROI** to the clipboard. This command is only used to select the **ROI** on the **Background Layer**.

Choosing the **Edit>Image Select** command will check this menu (or click  on the toolbar will keep  down) and the cursor will turn into "✚". The ROI selection steps are described as below:

1. After the **Edit>Image Select** command is chosen (or click the **Image Select** button  on the toolbar), the **Background Layer** will be checked automatically regardless of if the other **Layer** is checked or not;
2. Drag the mouse cursor across the image with the left button held down until the area is selected;
3. Release the left button and the area will be marked. Handles will appear on the area that will allow altering the selection after it is marked.

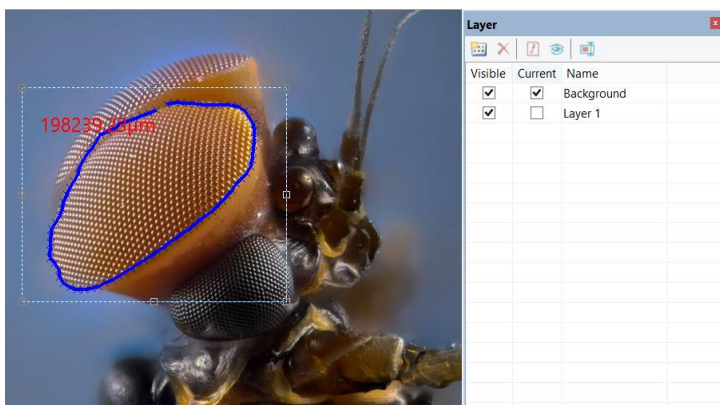

## 7.7 Select All(A)      Ctrl+A

### 7.7.1 Select all on the background layer

When the video/image window is active and the [Background Layer](#) is checked, choosing the [Select All](#) command will select all pixels on the [Background Layer](#) within the canvas (shortcut: [Ctrl+A](#)).

### 7.7.2 Select all objects over the background layer

When the video/image window is active and the [Background Layer](#) is not checked, choosing the [Edit>Select All](#) command will select all of the [Objects](#) on the [Current Layer](#) (shortcut: [Ctrl+A](#)).

### 7.7.3 Select all files in the Browse window

When the [Browse](#) window is active, choosing the [Edit>Select All](#) command will select all of the files in the [Browse](#) window under the specified directory in the [Folders Sidebar](#).

## 7.8 Select None(N)      Ctrl+D

Deselect a) any selected area (ROI) on the image; b) the [Objects](#) on a Layer; c) the file listed in the [Browse](#) window.

### 7.8.1 Select None for Background Layer

When the [Current Layer](#) is the [Background Layer](#) and an image area is selected, the [Select None](#) menu will be enabled. Choosing the [Edit>Select None](#) command will delete the dotted rectangle representing the selected area (ROI).

### 7.8.2 Select None for Objects

When the [Current Layer](#) is not the [Background Layer](#) and the [Objects](#) are selected, the [Edit>Select None](#) command will be enabled. Choosing the [Edit>Select None](#) command will deselect all of the selected [Objects](#).

### 7.8.3 Select None for Browse window

When the [Browse](#) window is active and the image files in the browse window are selected, the [Edit>Select None](#) command will be enabled. Choosing the [Edit>Select None](#) command will deselect all of the selected files in the [Browse](#) window.

**Note:** See [Edit>Image Select](#), [Edit>Select All](#) and [Measurements>Object Select](#)  to understand how to perform select operations.




## 8 View

### 8.1 Browse(B)



Ctrl+B

#### 8.1.1 Open the Browse window


1. Choose the [View>Browse](#) menu or click the [Browse](#) toolbar button  open or active browse images under the specified directory in the [Folders Sidebar](#);
2. Click the [Folders Sidebar](#) to activate it and double-clicking the listed directory in the [Folders Sidebar](#) will create the [Browse](#) window.

After creating the [Browse](#) window, [ImageView](#) will display a [Browse](#) window that looks like windows explorer. The child window on the left part of the [Browse](#) window called [Folders Sidebar](#) is used to locate the directory on the hard disk. Images in the current directory are displayed in [Large Icons](#) or [Small Icons](#) mode on the right side of the [Browse](#) window.

Image file's order can be set in [Ascending](#) or [Descending](#) order according to [Sort](#) by [Name](#), [Type](#), [Size](#), [Width](#) or [Height](#) et al.

#### 8.1.2 Browse window right mouse button context menu

Clicking the right mouse button on the listed [Icon](#) in the [Browse](#) window will bring up a right mouse button context menu as shown below:

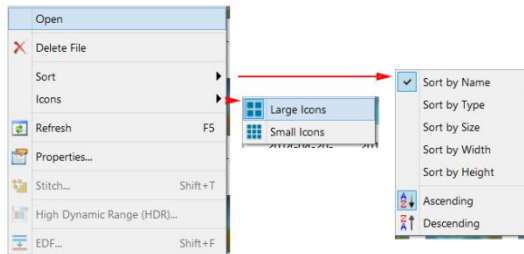

These context menu functions are described in

[Browse>Delete File](#)

[Browse >Sort>Sort by Names](#)

[Browse >Sort>Sort by Type](#)

[Browse >Sort>Sort by Size](#)

[Browse >Sort>Sort by Width](#)

[Browse >Sort>Sort by Height](#)


- Browse >Sort>Forward
- Browse >Sort>Reverse
- Browse >Icon>Large Icons
- Browse >Icon>Small Icons
- Browse >Refresh
- Browse >Properties

menus. Please check them for details.

There other menu can be found in [Process](#) menu in Sec.13.

**Note:** The [Folders Sidebar](#) and the [Browse](#) can be used to perform tasks such as creating new folders, renaming, moving, and deleting files. Individual file information and import data from digital cameras can also be displayed. Double-clicking the left mouse button on the icon will open the image as an active image in full size. See [Image window GUI](#) in Sec.3 for more details.

## 8.2 Measurement Sheet(M)

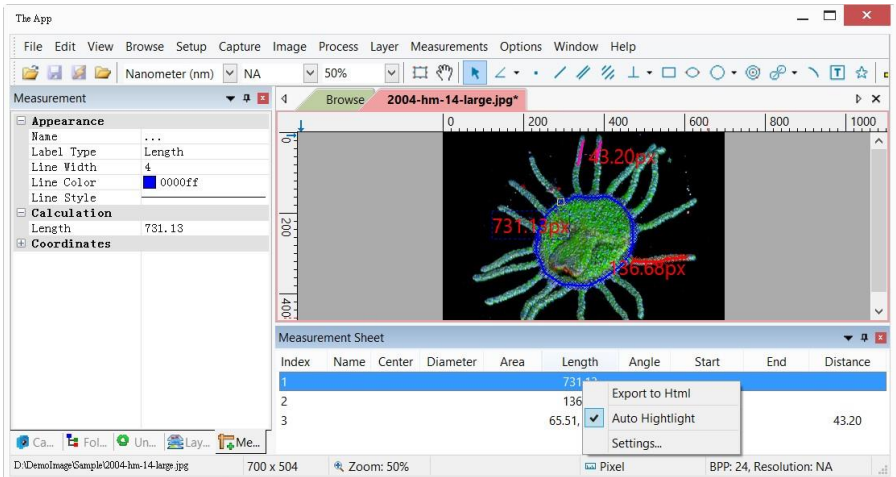

When choosing the [View>Measurement Sheet](#) command, the [Measurement Sheet](#) will be active. The [Measurement Sheet](#) shows the [Object's](#) possible features, such as [Name](#), [Center](#), [Radius](#), [Area](#), [Perimeter](#), [Angle](#), [Start Point](#), and [End Point](#) overlaid on [Background Layer](#).

Clicking the right mouse button on the [Measurement Sheet...](#) and the right mouse context menu will bring up on the [Measurement Sheet...](#) window as shown above. They are explained below:

### 8.2.1 Export Html

Export all the [Layer Objects](#) to the [\\*.html](#) file in a tabbed format.

Layer Name	Index	Name	Center	Diameter	Area	Length	Angle	Start	End	Distance
Layer1	1		(124.86, 239.18)	218.54	37509.04	686.55				
	1		(578.19, 249.50)	205.15	33055.73	644.51				
Layer2	2		(350.50, 246.50)			457.13	178.62	(579.00, 252.00)	(122.00, 241.00)	

Length Unit:Pixel, Angle Unit:Pi

**Note:** This menu will be enabled only when there are [Objects](#) overlaid on the [Background Layer](#) (video/image).

### 8.2.2 Auto Highlight


When this menu is checked, clicking the item in the [Measurement Sheet](#) will highlight the corresponding [Object](#) overlaid on the [Background Layer](#).

### 8.2.3 Settings...

1. To modify the [Measurement Sheet](#)'s item order, click the item to highlight it, the [Up](#) or [Down](#) button will be enabled (If the item is in the third position, the [Up](#) button will be disabled, if the item is in the last row, the [Down](#) button will be disabled). Click the [Up](#) or [Down](#) button to modify the item order;
2. Checking/Unchecking the item will show/hide the item in the [Measurement Sheet](#);
3. Clicking [Default](#) will return to the [ImageView's](#) default settings;
4. Item 1([Index](#)) and item 2([Name](#)) cannot be changed (in grayed state).

**Note:** The item [Index](#) and [Name](#) are always in grayed states, this means these two items cannot be modified (Both their hide/show states and their positions).


# Edit

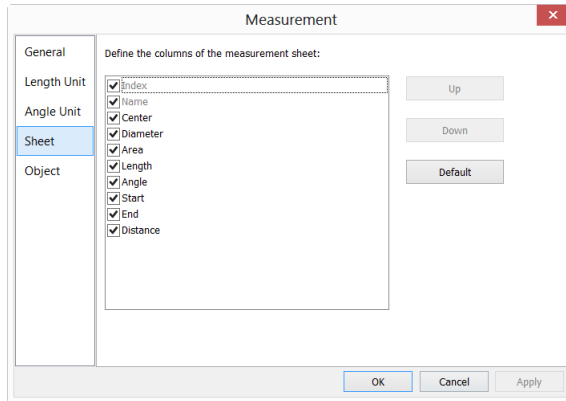

## 8.3 Sidebar

There are 5 Sidebar in the **ImageView** frame window in tabbed style. They are **Camera Sidebar**, **Folders Sidebar**, **Undo/Redo Sidebar**, **Layer Sidebar** and **Measurement Sidebar**.

### 8.3.1 Sidebar overview

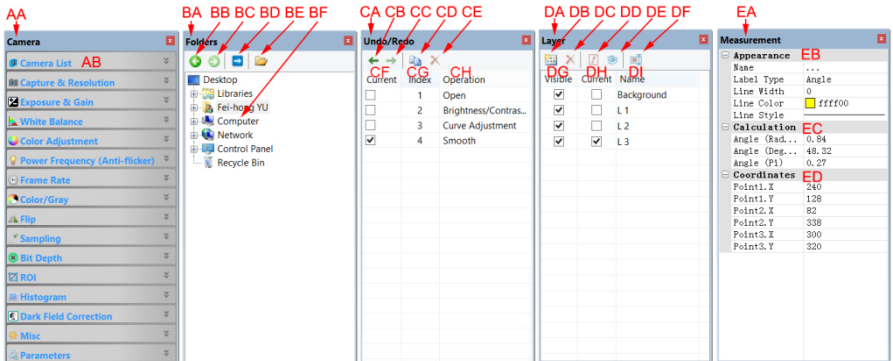

AA: **Camera Sidebar**;

AB: **Camera Sidebar** groups for the control of the camera.

BA: **Folders Sidebar**;

BB: **Back** to the previous folder;

BC: **Forward** to the next folder;

BD: **Browsing** the pictures under the application's file directory;

BE: Open the **Browse** window if it is not opened (Double-clicking on the selected

directory will perform the same functions.);

BF: [Folders](#) to locate the [Browse](#) window's file directory.

CA: [Undo/Redo Sidebar](#);

CB: Forward to the previous step;

CC: Backward to the next step;

CD: [Operation Copy](#): Copy the highlighted operation in the [Undo/Redo Sidebar](#) to a new image window; User can also drag the selected operation in the [Undo/Redo Sidebar](#) to the window area to create a new image window;

CE: [Remove](#) the highlighted operations from the [Undo/Redo](#) list (This button will be enabled only when the operation(s) is (are) selected, the opened image(the first operation) cannot be removed;

CF: Indicating the [Current](#) operation displayed in the image window;

CG: [Operation Index](#);

CH: [Operation](#) name.

DA: [Layer Sidebar](#);

DB: Make a [New](#) layer;

DC: [Remove](#) a layer;

DD: Set as the [Current](#) layer;

DE: [Show/Hide](#) a layer;

DF: [Rename](#) a layer;

DG: Visibility control of the layer items;

DH: The [Current](#) active layer for operations;

DI: The layer [Name](#). The image layer is always named as "[Background](#)".

EA: [Measurement Sidebar](#);

EB: The [Appearance](#) of the highlighted [Object](#) on the [Current](#) layer; you can edit the [Appearance](#) by clicking its item and editing it;

EC: The [Calculation](#) of the highlighted item on the [Current](#) layer;

ED: The [Coordinate](#) of the highlighted item on the [Current](#) layer; you can edit the [Coordinate](#) by clicking the item.

### 8.3.2 Sidebar>Camera(C)

The [Camera Sidebar](#) is mainly used for the control of camera, it includes many groups. Each group can be expanded by clicking the group name or the arrow button

at the right of the group name.

Checking the [Sidebar>Camera](#) menu will activate/show it on sidebar group.

Please check [Camera Sidebar](#) in Sec.5 for details.

### 8.3.3 Sidebar>Folders(F)

The [Folders Sidebar](#) is mainly used for the image [Browse](#) control.


Checking the [View >Sidebar>Folders](#) menu will activate/show the [Folders Sidebar](#).

Clicking its tree can navigate the file directories.

Double-clicking the directory in the [Folders](#) will create the [Browse](#) window. If there are image files under the directory that [ImageView](#) supports to [Browse](#), the image files will be displayed in [Large](#) or [Small](#) icons mode.

Their orders can be set in [Ascending](#) or [Descending](#) styles according to [Sort](#) by [Name](#), [Type](#), [Size](#), [Width](#) or [Height](#) et al.

Clicking the right mouse button on the directory will bring up the right mouse context menu as shown below:

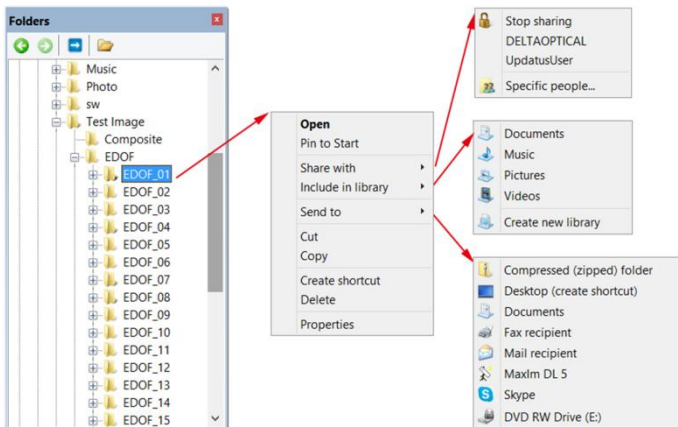

Folders directory right mouse button context menu

This is the basic window explorer menu and will not be explained in this manual.

### 8.3.4 Sidebar>Undo/Redo(U)

The [Undo/Redo Sidebar](#) is used to list the [Undo/Redo](#) operations for the [Image](#) and [Process](#) menus' command.

Checking the [View>Sidebar>Undo/Redo](#) menu will activate/show the [Undo/Redo Sidebar](#).

### 8.3.5 Sidebar>Layer(L)

[Layer Sidebar](#) is used for the management of [Layer](#) operations. These operations include making a [New Layer](#), [Removing](#) a [Layer](#) or [Renaming](#) a [Layer](#) and [Layer](#) visibility controlling et al.

Checking [View>Sidebar>Layer](#) will activate/show the [Layer Sidebar](#).

### 8.3.6 Sidebar>Measurement(M)

The [Measurement Sidebar](#) is used to check or edit the selected [Objects](#) on the [Layer](#).

Checking [View>Sidebar>Measurement](#) will activate/show the [Measurement Sidebar](#).

In this sidebar, the [Object Appearance](#), [Calculation](#) and [Coordinates](#) characteristic are listed. The [Appearance](#) and [Coordinates](#) can be edited.

## 8.4 Grid(G)

The [Grid](#) menu has 5 submenus, they are:

### 8.4.1 Settings(S)●●●




Choosing the [View>Grid>Setting●●●](#) command, or choosing the [Preference>●●●](#) command and clicking the [Grids](#) page realize the same function.

Choosing the [Preference>●●●](#) command and clicking the [Grids](#) page can set the [Grid Style](#), [Line Style](#), and [Line Color](#) for the [Grid](#) overlaid on the video and image window can also be set.

**Style:** The [Grid Style](#) can be [No Grid](#), [Auto Grid](#) or [Manual Grid](#). Default is [No Grid](#);

**Line Style:** The [Line Style](#) for the grid can be [Solid](#), [Dash](#), [Dot](#) or [DashDot](#) et al. Default is [Solid](#);

**Color:** The color of the grid line. Default is Red (255,0,0).

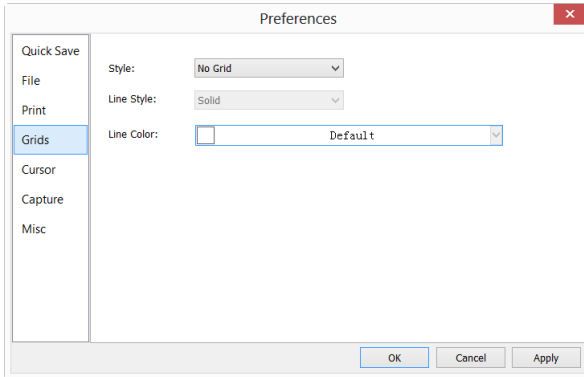

### 8.4.2 Grids>No Grids(N)

Choosing this command will remove both [Manual Grids](#) and [Auto Grids](#) overlaid on the video/image window.

### 8.4.3 Grids>Auto Grids(A)

Choose [Grids>Auto Grids](#) command to overlay the grids on the video/image automatically.

The [Auto Grids](#) can be set in the [View>Grids>Setting•••](#) menu.

### 8.4.4 Grids>Manual Grids(M)

Choosing this command will display two small [Right Arrow](#) and [Down Arrow](#) overlaid on the top of the [Vertical Ruler](#) and on the left of the [Horizontal Ruler](#) as shown below:


[Down Arrow](#): Move the mouse over the [Down Arrow](#) will show a horizontal drag icon. Drag the [Down Arrow](#) along the [Horizontal Ruler](#) to where ever you want. When it is dragging over the video/image, there will be a [Vertical](#) line appeared to let you judge where to release this line on the video/image. You can drag any lines to overlay them on the video/image.

The overlaid lines can be adjusted by dragging the specific [Down Arrow](#) again on [Horizontal Ruler](#).


[Right Arrow](#): Move the mouse over the [Right Arrow](#) will show a vertical drag icon. Drag the [Right Arrow](#) along the [Horizontal Ruler](#) to where ever you want. When it is dragging over the video/image, there will be a [Horizontal](#) line appeared to let you



judge where to release this line on the video/image. You can drag any lines to overlay them on the video/image.

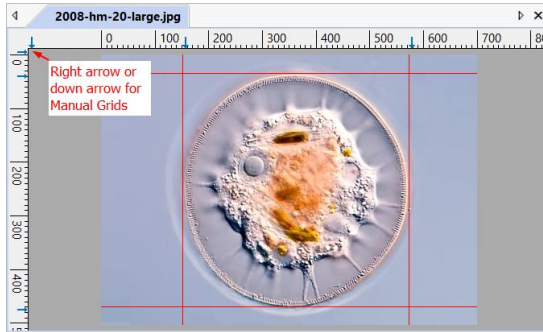

The overlaid lines can be adjusted by dragging the specific **Right Arrow** again on **Vertical Ruler**.

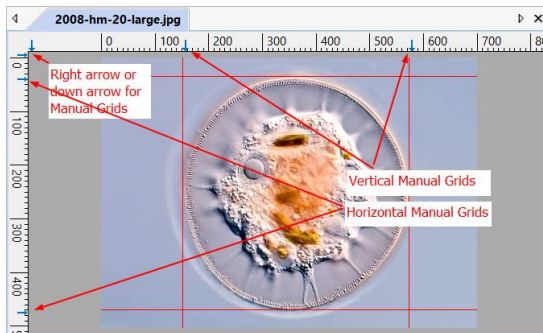

Choose the **Grids>No Grid** command to remove the **Manual Grids** overlaid on the video/image window. The menu will be checked.

Choose the **Grids>Manual Grids** command again (If it is unchecked) to display all the previous **Manual Grids** overlaid on the video/image window. The menu will be checked.

#### **8.4.5 Grids>Remove All Grids(R)**

Remove (Delete) all of the **Manual Grids** or **Auto Grids** overlaid on the image/video window.

#### **8.5 Best Fit(E) Num \***

Choose **View>Best Fit** command to automatically resize the video/image to fit in the

window.

**Note:** Choosing this command will enable [View>Actual Size](#) menu.

### **8.6 Actual Size(A)          Num /**

**Note:** This option will be disabled if the image is currently viewed at 100%. At any other zoom ratio, [View>Actual Size](#) will be enabled.

Choose [View>Actual Size](#) command to set the active image to its [Actual Size](#) (e.g. 100%).


### **8.7 Full Screen(F)                   ESC**

Choosing the [View>Full Screen](#) command will display the video window in full screen style. Press the [ESC](#) button will restore the video window.

### **8.8 Track(K)**

**Note:** If the video/image size is smaller than the window size. The track operation will be disabled.

If the image's actual size is larger than the video/image window, check this command to position the video/image that does not fit entirely within in the video/image window. Its function is similar to the scroll bars. It is an alternative to using the arrows on the scroll bars for positioning the video/image within the window.

Checking the [View>Track](#) menu will change the cursor to  and the button on the toolbar will be checked.

Then keep down the mouse button to drag the region of interest on the video/image to any location in the video/image window.

## 9 Browse

### 9.1 Sort(S)

#### 9.1.1 Sort>Sort by Names(N)

This command is for the [Browse](#) window only.

[Sort](#) the image files in order of names in the [Browse](#) window.

#### 9.1.2 Sort>Sort by Type(T)

This command is for the [Browse](#) window only.

[Sort](#) the image files in order of file type in the [Browse](#) window.

#### 9.1.3 Sort>Sort by Size(S)

This command is for the [Browse](#) window only.

[Sort](#) the image files in order of file size in the [Browse](#) window.

#### 9.1.4 Sort>Sort by Width(W)

This command is for the [Browse](#) window only.

[Sort](#) the image files in order of image file width in the [Browse](#) window.

#### 9.1.5 Sort>Sort by Height(H)

This command is for the [Browse](#) window only.

[Sort](#) the image files in order of image file height in the [Browse](#) window.

#### 9.1.6 Sort>Ascending(A)



This command is for the [Browse](#) window only.

[Sort](#) the image files in order of the [Ascending](#) mode (i.e. 1, 2, 3 and 4) in the [Browse](#) window.

#### 9.1.7 Sort>Descending(D)



This command is for the [Browse](#) window only.

[Sort](#) the image files in order of the [Descending](#) mode (i.e. 4, 3, 2 and 1) in the [Browse](#) window.

The [Sort](#) settings are saved until they are changed. For example, if you sort images in the [Browse](#) window according to the [Type](#), the images will remain sorted according to

Type until the [Sort](#) settings are changed.

## 9.2 Icon(I)

### 9.2.1 Icon>Large Icons(L)



This command is for the [Browse](#) window only.

The [Thumbnail](#) mode displays small preview images; you can select different view modes in the [Browse](#) window.

Choosing the [Icons>Large Icons](#) will display the image files in [Large Icon](#) mode in the [Browse](#) window.

### 9.2.2 Icon>Small Icons(S)



This command is for the [Browse](#) window only.

The [Thumbnail](#) mode displays small preview images; you can select different view modes in the [Browse](#) window.

Choosing the [Icons>Small Icons](#) will display the image files in [Small Icon](#) mode in the [Browse](#) window.

## 9.3 Refresh(R)



**F5**

This command is for the [Browse](#) window only.


If the files under the [Folders Sidebar](#)'s directory are altered outside of [ImageView](#), after switch back to [ImageView](#), one can [Refresh](#) the image files in the current directory to update the [Thumbnails](#) with [Browse>Refresh](#) command.

## 9.4 Properties(P)●●●



If an image file listed in the [Browse](#) window is highlighted. Choosing the [Browse >Properties](#) command or clicking the selected file in the [Browse](#) window with the right mouse button context menu [Properties](#) will bring up a [Properties](#) dialog as shown below:

## Browse

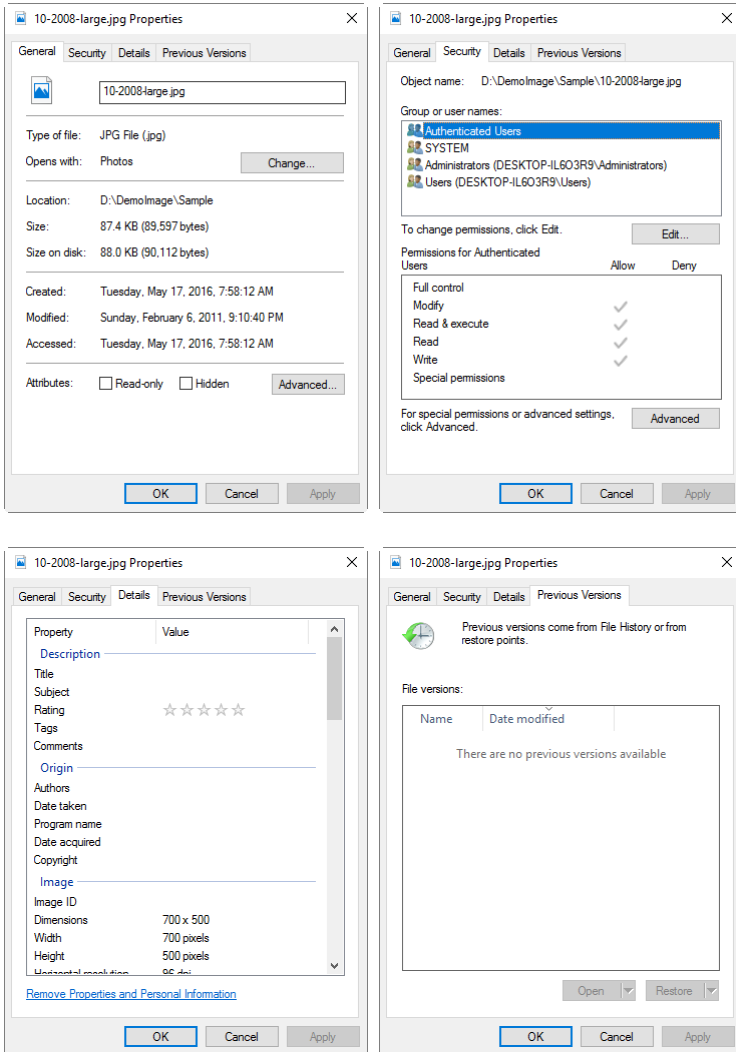

The file **Properties** dialog including 3 pages. They are **General**, **Security** and **Details** pages. These **Property pages** may depend on the operating system and we will not discuss it in this help manual.

## 10 Setup

### 10.1 Start/Pause(U)




Pause

If the video in video window is playing, one can choose the [Setup>Start/Pause](#) command to pause the video and choose the [Setup>Start/Pause](#) command again to start the video again.

### 10.2 View Properties(V)●●●

Shift+V

The [Setup>View Property●●●](#) will help you to understand the camera statistical properties. Choose the [Setup>View Property●●●](#) command to invoke the [View Property](#) dialog as below:

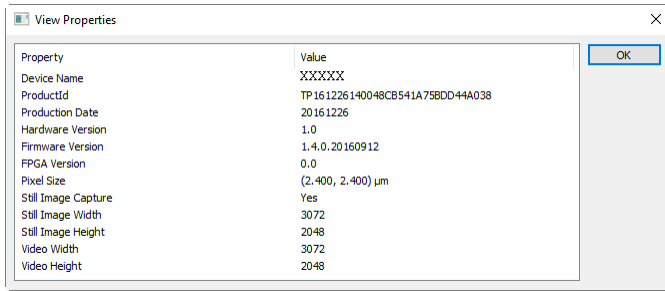

The items in the dialog are described in the following table:

**Device Name:** Readable string to identify the name of the camera device;

**ProductId:** Unique ID to identify the camera device;

**Still Image Capture:** To identify whether or not the camera supports [Still Image Capture](#). [Still Image Capture](#) is used for high resolution camera to capture an image with a different resolution from the video. This feature is mainly used to capture high resolution image under low resolution video to compromise between the frame speed and the image resolution;

**Still Image Width:** The to be captured image width;

**Still Image Height:** The to be captured image height;

**Video Width:** The actual video window video width;

**Video Height:** The actual video window video height;

**Time (second):** Seconds elapsed after the camera video has been started;



**Frame:** Frames acquired after the video has been started;

**Actual Frame Rate:** The camera frame rate of the video stream, which is the **Frame by Time**.

### 10.3 Video Overlay(O)●●●

#### 10.3.1 Video Overlay>Overlay

Choose the **Setup>Video Overlay●●●** command, this will invoke a **Video Overlay** dialog. Click the **Overlay** page on the **Video Overlay** dialog can set **Scale**, **Magnification**, **Date Time** and **Clarity Factor** to overlay on the video window.

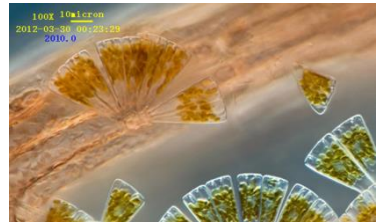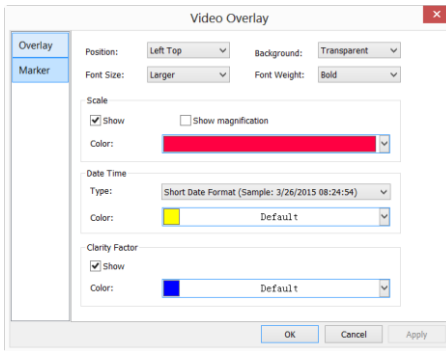

The **Position**, **Background**, **Font Size**, **Font Weight** of the **Scale**, **Magnification** and **Date Time**, and **Clarity Factor** can be defined together. Their **Colors** can be defined separately.

Clicking the **OK** button and the **Scale**, **Magnification** and **Date Time**, and **Clarity Factor** will be overlaid on the **Video** window.

The **Clarity Factor** can tell if the sample is in good focused state or not. The larger the **Clarity Factor**, the better the sample focused.


**Note:** To enable the **Scale** bar, the **Magnification** must be defined and chosen first in the **Unit** combo box on the toolbar. The **Unit** can be any unit except **Pixel**. There are two methods to set the **Unit**, they are: a) Choosing the **Unit** in the **Unit** dropdown combobox ( Micrometer (µm) NA 400% ) on the toolbar which is just on the left of the **Magnification** dropdown list box; b) Choosing the **Option>Measurement●●●** command, a dialog called **Measurement** will bring up, click the **Length Unit** page and check the **Unit** in the **Current** to set the **Unit**.

#### 10.3.2 Video Overlay>Marker●●●


## Setup

Choose the [Setup>Video Overlay...](#) command, this will invoke a [Video Overlay](#) dialog. Click the [Marker](#) page on the [Video Overlay](#) dialog to set the [Marker](#) on the video window.

The [Video Marker](#) type can be [None](#), [Cross](#), [Rectangle](#), [Circle](#), [Cross+Rectangle](#), or [Cross+Circle](#). The [Video Marker](#) page is shown as below:

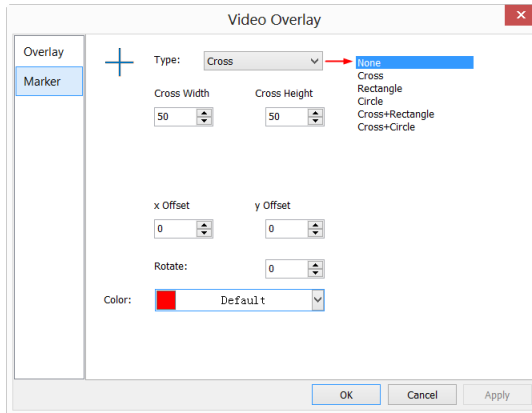

Choosing "[Cross+Rectangle](#)" in the [Type](#) combobox and [Video Overlay: Marker](#) dialog will change to the following style:

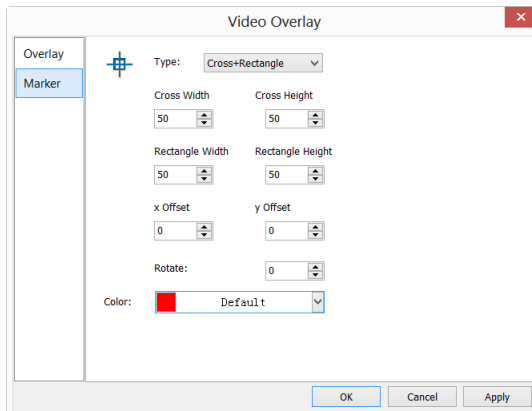


Edit the [Cross Width](#) and [Cross Height](#), [Rectangle Width](#) and [Rectangle Height](#), [x Offset](#) and [y Offset](#), in their specific fields. Click [Color](#) to define the [Video Marker](#) color.



## Setup


Click **OK** to end the **Video Marker** setup page and a **Cross+Rectangle Marker** will be overlaid on the video window as shown below:


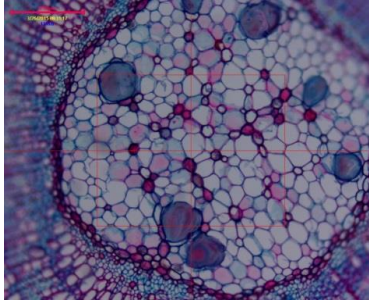


Click **Cancel** to cancel the **Video>Overlay: Marker** setup and return to the application area, or **Apply** to overlay the **Marker** on the video window and keep the **Video Overlay** dialog there for further setup.


### 10.4 Video Watermark(W)●●●

Fig.1 shows a **micro ruler**. The dark lines can be extracted as **Video Watermark** and overlaid on the video window. The steps are as follows:

1. Choose the **Capture>Capture Image** command or click  to capture the **micro ruler** image as shown in Fig.1;
2. Choose the **Process>Binary●●●** command to binarize the image as shown in Fig.2;
3. Choose the **Image>Adjust>Invert** command to invert the image and choose the **Image>Color Quantize●●●** command to convert the image to 24 bits as shown in Fig.3. Choose the **File>Save As●●●** command to save the image in **24 bit BMP** format;

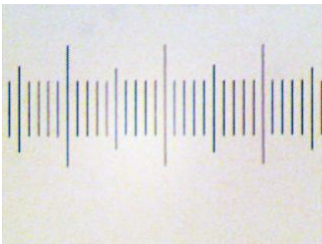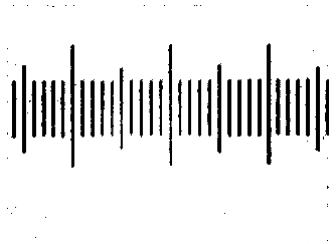	
Fig.1 Captured <b>Micro Ruler</b>	Fig.2 <b>Micro ruler</b> after being binarized

## Setup

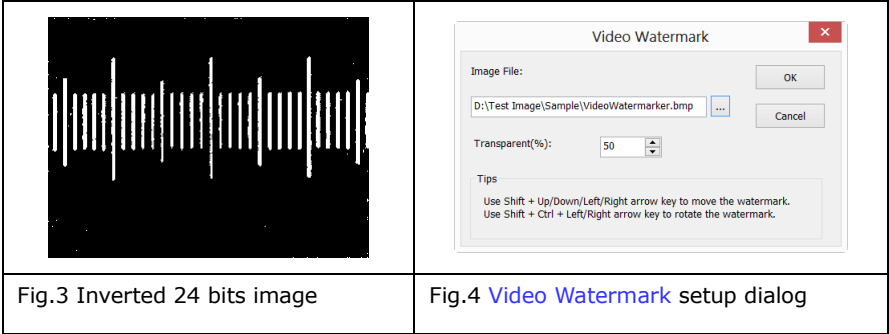

4. Choosing the **Setup>Video Watermark** command and a dialog called **Video Watermark** is brought up as shown in Fig.4. Click the **...** button to locate the image saved in step 3. Use the defaults **Transparent (%)**(50). If everything is ok, click **OK** button. The final **Video Watermark** is overlaid on the video window as shown in Fig.5.

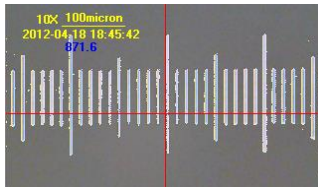



Fig.5 Video Window with Video Watermark overlaid

### 10.5 Move Watermark(M)

#### 10.5.1 Move to(W)

If there is **Watermark** overlaid on the video window, this menu will be enabled.

Choosing the **Setup>Move Watermark** command will bring up a **Move** dialog. Where one can enter the **X:** and **Y:** offset value in their fields for the desired pixel move distances. The default **X** and **Y** offsets are 0;

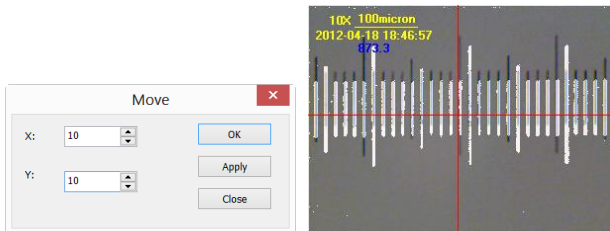

#### 10.5.2 Move to zero

If the **Watermark** on the video window was moved, this menu will be enabled.


Choosing this menu will move the **Video Watermark** to its original coordinates (0, 0).

### 10.6 Rotate Watermark®

#### 10.6.1 Rotate to(R)●●●

If there is **Watermark** overlaid on the video window, this menu will be enabled.

Choosing the **Setup>Rotate Watermark>Rotate to●●●** command will bring up a **Rotate** dialog, where one can define an **Angle** to **Rotate** the **Video Watermark** a specified angle around the video center (0, 0) (default value).

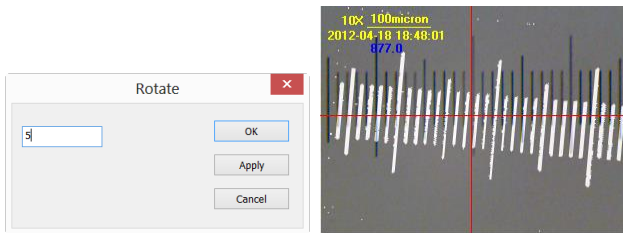

#### 10.6.2 Rotate to zero


If the **Video Watermark** was rotated, the **Rotate to zero** menu will be enabled. Choosing this menu will rotate the **Video Watermark** to zero degree.


### 10.7 Gray Calibration(G)●●●



This function can make the image brightness to a desired value among various scenarios in a specified area, achieving the continuity requirement of the observation. The **Gray Calibration** steps are summarized as follows:

1. Click the **Exposure & Gain** group name on the **Camera Sidebar** to expand the **Exposure & Gain** group, uncheck the **Auto Exposure** box (If it is checked).

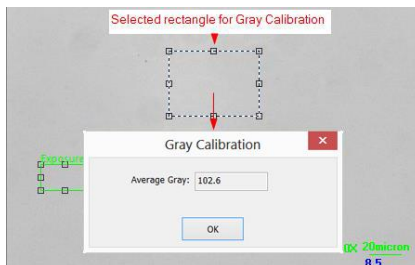

2. Choose the **Edit>Image Select** command or click the **Image Select** button  on the toolbar to select a reference region, and choose the **Setup>Gray Calibration●●●**

## Setup

---

command. A dialog called [Gray Calibration](#) will be brought up to display the current [ROI Average Gray](#). Now the brightness of the microscope can be adjusted until the [Average Gray](#) reaches to the desired value. Click "OK" to finish the calibration and return to the application area. The current gray value here is around is 102.

## 11 Capture


### 11.1 Capture Image(C)



F8

During the video preview, you can always choose the [Capture>Image Capture](#) command to capture the video image.


After the image is captured, the captured image will become the current active window. The [Capture>Capture Image](#) menu will be disabled. If you wish to capture image again, click the video window title to activate the video window and the [Capture>Capture Image](#) menu will be enabled again.

**Note:** a) The “Snap” button  on the [Camera Sidebar](#) can continuously snap the image even if the video window is not activated. User can click this button on the [Camera Sidebar](#) to capture image in quick style; b) Only when the video window is active, the [Capture>Capture Image](#) menu will be enabled; c) If the [Live](#) and [Snap](#) resolutions are different, [ImageView](#) need to switch the resolution from [Live](#) to [Snap](#) resolution in the backstage to capture an image with [Snap](#) resolution. After the [Snap](#) is finished, [ImageView](#) will switch back to the [Live](#) resolution to continue the video stream process. This will take more time to capture a still image.

### 11.2 Start Time-lapse (Auto Capture)●●●



Choosing the “[Capture>Start Time-lapse \(Auto Capture\)●●●](#)” command will bring up [Time-lapse \(Auto Capture\)](#) dialog shown below:

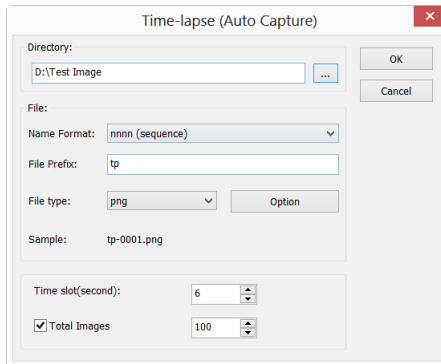

This function can capture a sequence of pictures with the specified time interval; you can precisely set the time interval (2 to 3600 seconds) and the total number of

images(1 to 9999).

**Directory:** The file [Directory](#) can be select by clicking on the [Browse](#) button;

**File:** The [File](#) name including [Name Format](#), [File Prefix](#), [File type](#). It can be a combination of [File Prefix](#), [Name Format](#) and [File Type](#) and is shown in the [Sample](#);

**Time Slot(Second):** [Time slot\(Second,2-3600S\)](#) is a time segment to capture an image;

**Total Images:** Checking [Total Images](#) will enable its edit box. You can enter the [Total Images](#) (1-9999) to be captured. [ImageView](#) will stop the [Time-lapse](#) capture process automatically when the [Total Images](#) are reached;


If [Total Images](#) is unchecked, [ImageView](#) will capture the images continuously until user choose the [Capture>Stop Time-lapse \(Auto capture\)](#) command again to stop the [Time-lapse](#) capture.

Click [OK](#) to begin the [Time-lapse](#) capture, or [Cancel](#) to cancel the [Start Time-lapse\(Auto Capture\)...](#) command.


After the [Time-lapse](#) capture is started, the [Capture>Start Time-lapse \(Auto Capture\)...](#) menu will be changed to the [Capture>Stop Time-lapse \(Auto capture\)](#) menu. Choosing this command will stop the [Time-lapse](#) capture.

There are a variety of image format available (they are [bmp](#), [jpg](#), [png](#) and [tif](#)) to save the captured image. For example, when choosing [jpg](#) format, you can set the parameters of "[Option](#)" to adjust its compression quality or encoding method. Please check the [File>Save As...](#) menu for these details.


### 11.3 Start Record(V) ... F9

1. You can a) choose the [Capture>Start Record...](#) command; b) click "[Record](#)" button  on the [Camera Sidebar](#) ; c) use the shortcut key "[F9](#)" to start recording movies. The will bring up a [Video File](#) dialog as below; Enter the video file name under [1.Set the name for the captured video file](#) field and click the [Browse...](#) button under [2 Select the directory for the video file](#) item to locate the video file directory. Click [Next](#) to the next step;

## Capture

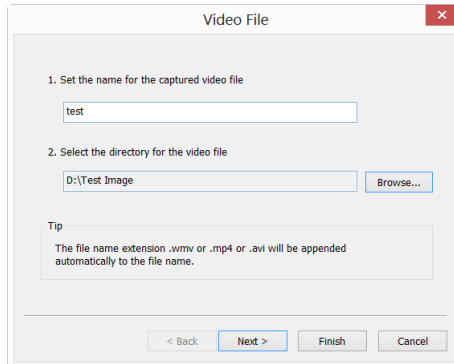


2. Clicking **Next** on the **Video File** dialog will display the **Video Format and Encoder** dialog. The video format can be **wmv/asf(recommended)** **H264(recommended)** or **avi**; Click **Back** to return to the **Video File** dialog, or **Next** to the next step;

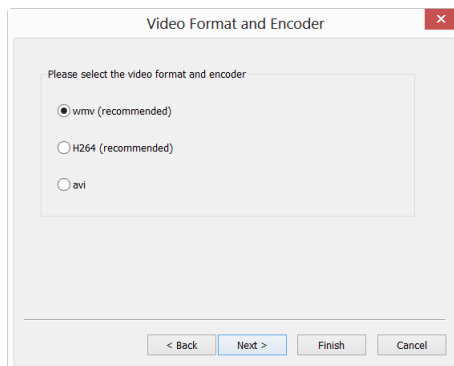




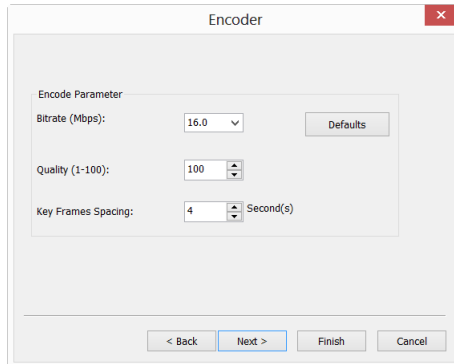


3. An **Encoder** dialog will be brought up. Here you can select the **Encoder** format, set the **Bitrat(Kbps)**(256-16384), **Quality** (1-100) and **Key Frames Spacing** (1-30). Click **Back** to return to the **Video Format** dialog, or **Next** to the next step;

## Capture

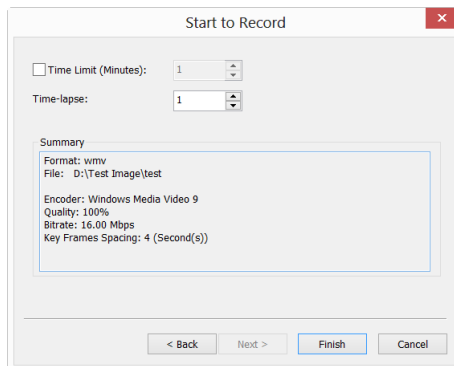

4. A dialog called **Start to Record** will be brought up. Here you can check **Time Limit (Minutes 1-1440)** and enter recording time (If checked); Input **Time-lapse(1-100)**. There is a **Summary** text to display what you have been defined. Click **Back** to return to the **Encoder** dialog, or **Finish** to end the setup;



5. After the **Video** capture is started. The  **Record** button on the **Camera Sidebar** will become  . Clicking  will stop the capture process, otherwise ,it will stop until the **Time Limit** is reached. After the **Video** capture process is finished. The  on the **Camera Sidebar** will become  for the future **Record** process;

6. You can choose the **File>Open Video...** command to display the captured video




file in the video window;

### 11.4 Start Broadcast(B)●●●

Start a network broadcasting service. Select the [Port](#) and [Encoder](#) before start the service. After that, [ImageView](#) will start broadcasting the video that is opened by [ImageView](#) locally via the specified [Port](#) and [Encoder](#). The other users could share the video by open broadcasting function.


Choosing [Capture>Start Broadcast●●●](#) will invoke a [Broadcast Parameters](#) dialog as below:

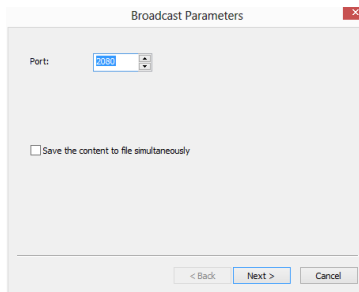

[Port](#): Set the [Port](#) and;

[Save the content to file simultaneously](#): Check or uncheck [Save the content to file simultaneously](#);

[Next>](#): Clicking the [Next>](#) button will invoke a [Encoder](#) dialog as shown below:

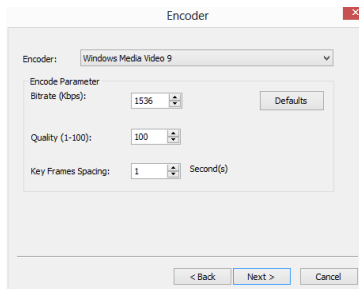


This dialog is used for the setup of video [Encoder](#) parameters for broadcasting. This setup dialog is just the same as those of [Capture>Start Record●●●](#) setup dialog. It mainly including [Encoder](#), [Encode Parameter](#) such as [Bitrate](#), [Quality\(1-100\)](#), [Key](#)

[Frame Spacing](#) in second et al.

**Next>**: Clicking the **Next>** button again will invoke the **Start to Broadcast** dialog. Here, one can set the broadcast **Time Limit** in minutes. The **Encoder** parameters are also listed in the Summary window for reference;

**<Back**: Clicking **<Back** will return to **Broadcast Parameters** dialog;

**Cancel**: Clicking will end the **Start Broadcast•••** command and return to the video window.

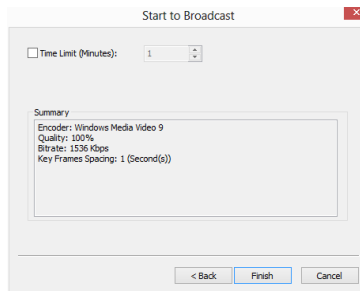

**<Back**: Clicking **<Back** will return to **Encoder** dialog;

**Cancel**: Clicking will end the **Start Broadcast•••** command and return to the video window;

**Finish**: Clicking the **Finish** button will start the broadcasting process and it will end up the process when it reaches to the **Time Limit**;

See **File>Open Broadcast•••** to understand the **Start Broadcast** function.


## 12 Image

### 12.1 Mode(M)

#### 12.1.1 Color Quantize(Q)●●●

The [Color Quantize](#)●●● command is widely used to change the image bit. [ImageView](#) supports the mutual changes among 24 bit, 8 bit, 4bit or 1 bit images.

When the [Colour Bits](#) dialog is opened, the default checked color bits is the current image's color bit. Check the desired bit and click [OK](#) to end the command. The image will converted to the selected color bits in the image window.




#### 12.1.2 Gray Scale(G)


Choose the [Gray Scale](#) command to convert a color image (true color image or index color image) to a gray scale image. If the original image is 24 bit, the new image is 8 bit. Otherwise the bits of the image will not be modified.

#### 12.1.3 Contrast Preserving Decolorization©


Choose the [Image>mode>Contrast Preserving Decolorization](#) command can convert the color image into gray image with contrast preserved. The following pictures (a) is the original microscopic image, (b) is the gray image produced by traditional method, (c) is the gray image produced by Contrast Preserving Decolorization.



(a) Original microscopic image

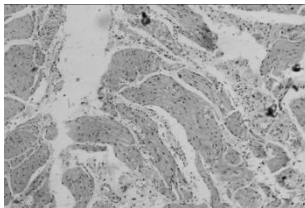

(b) Traditional method

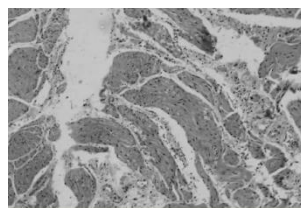


(c) Contrast Preserving Decolorization

## 12.2 Adjust(A)

### 12.2.1 Brightness/Contrast(A)●●●

The **Image>Adjustment>Brightness/Contrast●●●** command offers simple adjustments to the tonal range of an image. This command makes the same adjustment to every pixel in the image. The **Brightness/Contrast** command does not work with individual channels and is not recommended for high-end output because it can result in the loss of details about the image.

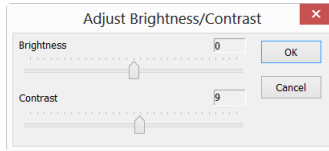


**Brightness:** Dragging the slider bar to the left decreases the level and dragging it to the right increases the level. The numbers on the right of the slider bar displays the **Brightness** value. Values can range from **-100** to **+100**. Default is 0;

**Contrast:** Dragging the slider bar to the left decreases the level and dragging it to the right increases the level. The numbers on the right of the slider bar displays the **Contrast** value. Values can range from **-100** to **+100**. Default is 0;

### 12.2.2 Color(O)●●●

Choose the **Image>Adjustment>Color●●●** command to modify the overall mixture of the colors in an image.

There are four color modules: **RGB**, **CMYK**, **HSI** and **HLS**.

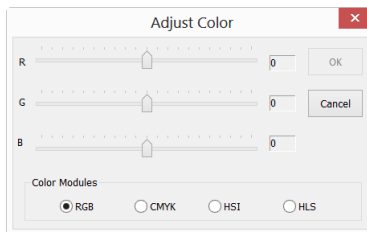


**RGB:** **ImageView** uses the **RGB** model. It assigns an intensity value to each pixel ranging from 0 (black) to 255 (white) for each of the **RGB** components in a color image.

For example, a bright red color might have an **R** value of 246, a **G** value of 20, and a

**B** value of 50. When the values of all three components are equal, the result is a shade of neutral gray. When the value of all components is 255, the result is pure white; when the value is 0, pure black.

**RGB** images use 3 channels to reproduce up to 16.7 million colors on-screen. In addition to being the default mode for new **ImageView** images, the **RGB** mode is used by computer monitors to display colors. This means that when working in color modes other than **RGB**, such as **CMYK**, **ImageView** uses **RGB** mode for display on-screen. Although **RGB** is a standard color mode, the exact range of colors represented can vary, depending on the application or display device.

**CMYK**: The **CMYK** mode is based on the light-absorbing quality of ink printed on papers. As white light strikes translucent inks, certain visible wavelengths are absorbed while others are reflected back to the eyes.

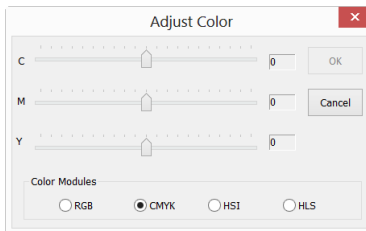


In theory, pure cyan (**C**), magenta (**M**), and yellow (**Y**) pigments should combine to absorb all light and produce black. For this reason these colors are called subtractive colors. Because all printing inks contain some impurities, these three inks actually produce a muddy brown and must be combined with black (**K**) ink to produce a true black. (**K** is used instead of **B** to avoid confusion with blue.) Combining these inks to reproduce color is called four-color process printing.

The subtractive (**CMY**) and additive (**RGB**) colors are complementary colors. Each pair of subtractive colors creates an additive color, and vice versa.

**HSI**: Based on the human perception of color, the **HSI** model describes 3 fundamental characteristics of colors:

## Image

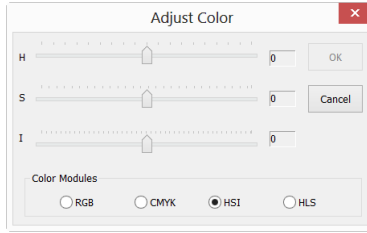


**Hue** is the color reflected from or transmitted through an object. It is measured as a location on the standard color wheel, expressed as a degree between  $0^\circ$  and  $360^\circ$ . In common use, **Hue** is identified by the name of the color such as red, orange, or green.

**Saturation**, sometimes called chroma, is the strength or purity of the color. **Saturation** represents the amount of gray in proportion to the hue, measured as a percentage from 0% (gray) to 100% (fully saturated). On the standard color wheel, **Saturation** increases from the center to the edge.

**Intensity** is the relative lightness or darkness of the color, usually measured as a percentage from 0% (black) to 100% (white).

**HLS**: The **HLS** model is very similar to the **HLS** color model. The main difference between them is the calculation used to produce the brightness value. In the **HLS** model, a pixel's brightness (**L**) is derived from its three (**R**, **G** and **B**) color values. In the **HLS** model, a pixel's brightness (**L**) is determined by the minimum and maximum values of its three color values.

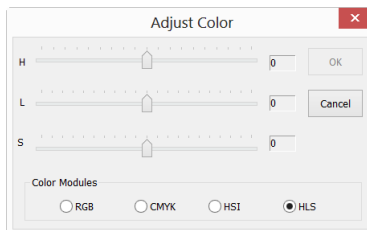

The values beside the slider bar show the color changes in various color channels.

For **RGB** channel values, they are range from **-100** to **+100**. Default is 0;

For **CMYK** channel values, they are range from **-100** to **+100**. Default is 0;


## Image

For **HSI** channel values, the **H** value can range from **-180** to **180**, the **S** value is range from **-275** to **275**, and the **I** value is range from **-442** to **442**. Default is 0;

For **HLS** channel values, the **H** value is range from **-180** to **180**, the **L** value is range from **-100** to **100**, and the **S** value is range from **-100** to **100**. Default is 0;


### 12.2.3 HMS●●●

Choose the **Image>Adjustment>HMS●●●** command to adjust the **HL** (Highlight), **M** (Midtone), and **S**(Shadow) parts of the image. Each part's value ranges from **-100** to **100**. This command is only available for 24 bits true color image.

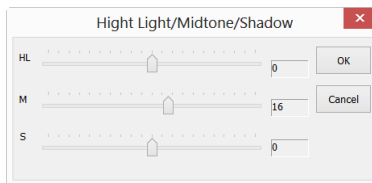

### 12.2.4 Curve(U)●●●

Choose the **Image>Adjust>Curve●●●** to adjust the entire tonal range of an image. But instead of making adjustments using only three variables (**Highlight**, **Midtone**, **Shadow**), one can adjust any point on the curve along a 0-255 scale while keeping up to any other values constant. One can also use **Curve** to make precise adjustments for individual color channels on an image. The **Curve** dialog is shown below:

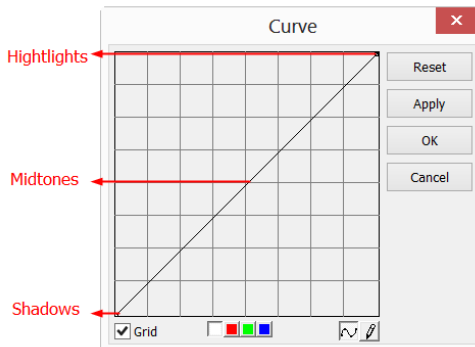

**Horizontal Axis:** The horizontal axis of the graph represents the original intensity values of the pixels (**Input** levels).

**Vertical Axis:** The vertical axis represents the new color values (**Output** levels). In the default diagonal line, all of the pixels have identical **Input** and **Output** values.

**Curve area:** Area (specified with the **blue rectangle**) to setup a map between input and output;

a) When you open the **Curve** dialog you see, perhaps surprisingly, not a curve but a straight line. As a default, the input values are the same as the output, so there's no change;

b) By clicking in the center of the line and dragging upwards, we make our first curve. Raising the curve increases the overall brightness of the scene.

c) Conversely, clicking in the center and dragging downwards lowers the brightness, producing an image that's darker overall;


d) As well as clicking in the center, we can also adjust the endpoints. Clicking the top right point and dragging down will limit the brightest part of the image, reducing contrast.

e) If we drag that top right point to the left rather than down, we produce the opposite effect—increasing the contrast of the image. This is a very useful and controllable quick fix;


f) By dragging the top and bottom points towards the center, we create a stylized, posterized effect that turns any photograph into more of a graphic object.

g) Click once in the center of the RGB curve to "pin" that midpoint; now drag just the top half of the curve to make this S shape, and the result is to increase the overall contrast.

h) You can add up to any control points to the curve, locking those values. To remove a control point, 1)drag it off the graph or 2)click the right mouse button on that point. You cannot delete the endpoints of the curve.

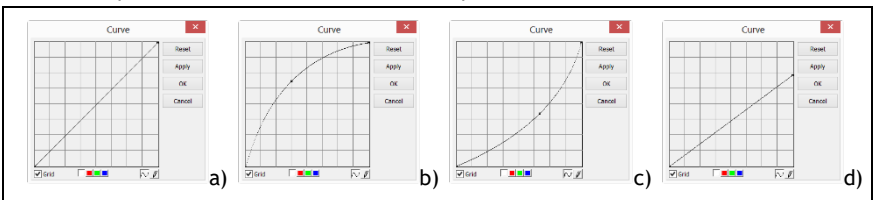



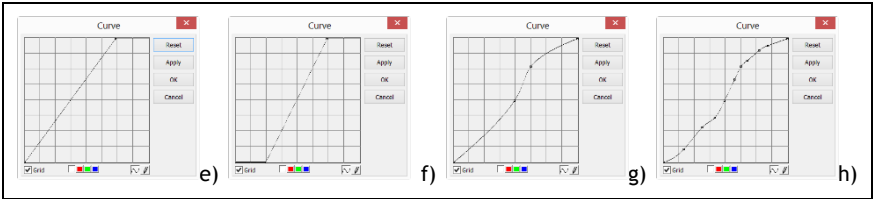



**Grid:** Check to overlay the grid on the **Curve** window;

**Channel**     : To adjust the color balance of the image, check the channel(R, G or B) from the **Channel** button. Check the white button to select RGB channels at the same time, which is located on the left of the R (Red), G (Green) and B (Blue) buttons;

**Curve** : Click the **Curve** with your left mouse button, a spline curve (straight line) will setup the initial input-output relation. Click on the **Curve** will mark the **Curve** with a point. The point number can be any as long as it can be inserted on the **Curve**. Drag the **marked point** until the image looks satisfactory. The point can be deleted by move the mouse on it and click the right mouse button on it.


**Pencil** : Check the pencil button at the bottom of the dialog, and use your left mouse button to draw a new arbitrary **Curve** in the **Curve** area.

**Reset:** Click the **Reset** button will reset the **Curve** to the initial straight line.

**Apply:** Apply current **Curve** map on the image.

### 12.2.5 Filter Color(F)●●●

Choose the **Image>Adjustment>Filter Color** command to filter a special color channel from a color image. Check either **Red**, or **Green**, or **Blue** color to filter. For every pixel, if check **Red** color to filter, only information about the red channel will be discarded, and **Green** and **Blue** information will remain there.




See **Image>Extract Color●●●** for another color operation.

## 12.2.6 Extract Color(E)●●●

Choose the [Image>Adjustment>Extract Color●●●](#) command to extract a special color channel from a color image. Check either [Red](#) or [Green](#), or [Blue](#) color to extract.

For every pixel, if selecting [Red](#) color to extract, only information about the red channel will be kept, and [Green](#) and [Blue](#) information will be discarded.



See [Image>Filter Color●●●](#) for another color operation.


## 12.2.7 Invert(I)

Choose the [Image>Adjustment>Invert](#) command to reverse the pixel values of the active image without going through the lookup table.

## 12.2.8 Edge Preserving Smooth(S)●●●

[Edge Preserving Smooth](#) is an image processing technique that smooth away textures whilst retaining sharp edges. Examples are the Bilateral filter, the Guided filter and Anisotropic diffusion.

Choose the [Image>Adjust>Edge Preserving Smooth●●●](#) command can smooth the entire image and preserve the edge of image, as shown below:

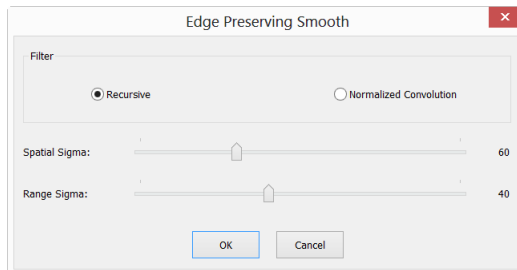


[Edge Preserving Smooth](#) function provide two kinds of filter including [Recursive](#) and [Normalized Convolution](#) filter, and the default filter is [Recursive](#).

[ImageView](#) use [Spatial Sigma](#) and [Range Sigma](#) to define the filter kernel size. The

bigger the two parameters, the stronger the image smoothed, vice versa.

### 12.2.9 Detail Enhance(D)●●●

Choose the **Image>Adjust>Detail Enhance●●●** command can enhance the detail in the image, as shown below:

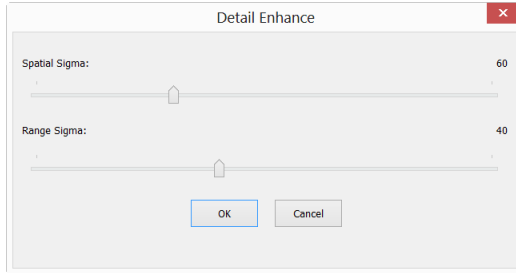

**ImageView** choose **Spatial Sigma** and **Range Sigma** to define the kernel size of detail enhance algorithm. The bigger the 2 parameters, the stronger the enhanced image and vice versa.

The following picture is the detail enhanced image for reference with default parameter.




a)Original image and b)Enhanced image

### 12.2.10 Auto Level(L)

The **Image>Adjustment>Auto Level** command moves the level's sliders automatically to set highlight and shadow. It defines the lightest and darkest pixels in each color channel as white and black and then redistributes the pixels' color values proportionately. Since **Auto Level** adjusts each color channel individually, it may remove or introduce color casts. The **Auto Level** command moves the level's

sliders automatically to set highlight and shadow. It defines the lightest and darkest pixels in each color channel as white and black and then redistributes the pixels' color values proportionately. Since [Auto Level](#) adjusts each color channel individually, it may remove or introduce color casts.

By default, this feature clips the white and black pixels by [0.5%](#)--that is, it ignores [0.5%](#) of the lightest pixels and [0.5%](#) of the darkest pixels when identifying the lightest and darkest pixels on the image. Choose the [Options>Auto Correction...](#) command to modify this default setting. This ensures that white and black values are representative without being determined by extreme pixel values. The [Auto>Correction...](#) dialog is shown below:



The [Image>Adjustment>Auto Level](#) command gives good results when an image with an average distribution of pixel values needs a simple contrast adjustment or when an image has an overall color cast. However, adjusting the [Curves](#) manually is more precise.


See [Image>Adjustment>Auto Contrast](#) for another auto adjust command.

### 12.2.11 Auto Contrast(T)

The [Image>Adjustment>Auto Contrast](#) command automatically adjusts the overall contrast and mixture of colors in an RGB image. Since it does not adjust channels individually, [Auto Contrast](#) does not introduce or remove color casts. It maps the lightest and darkest pixels in the image to white and black, which makes highlights appear lighter and shadows appear darker.

When identifying the lightest and darkest pixels on an image, [Auto Contrast](#) clips the white and black pixels by [0.5%](#)--that is, it ignores the first [0.5%](#) of either extreme.

Choose the [Options>Auto Correction...](#) menu to modify this default setting. This ensures that white and black values are representative without being determined by extreme pixel values. The [Auto Correction...](#) dialog is shown below:



The [Auto Contrast](#) command can improve the appearance of many photographic or continuous-tone images. It does not improve flat-color images.

See [Image>Adjustment>Auto Level](#) for another auto operation.

## 12.3 Rotate(R)

Choose the [Image>Rotate](#) command to rotate the entire image. One has the following submenus:

### 12.3.1 90(CW)

Rotate the image clockwise by a quarter-turn.

### 12.3.2 180(CW)


Rotate the image clockwise by 180 degrees.

### 12.3.3 270(CW)

Rotate the image clockwise by 270 degrees.

### 12.3.4 Arbitrary(A)●●●

Rotate the image by a specified angle. If choosing this option, enter an angle between 0 and 360 degrees in the angle text box, and check [CW](#) or [CCW](#) to rotate clockwise or counterclockwise. For the [Arbitrary●●●](#) operation, it will invoke an [Image Rotate](#) dialog like below:

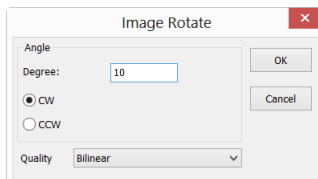

[Degree](#): The degree that the image to be rotated.

[CW](#): Rotates the image clockwise.

**CCW:** Rotates the image counterclockwise.

**Quality:** One can select one of the three methods for the image rotation among **Nearest Neighbor**, **Bilinear**, and **Bicubic**. The default is **Bilinear**.

### 12.3.5 Flip Horizontal(H)



Reverses the image in the application area so that the top right corner of the original image is now the top left, and the top left corner of the original image is now the top right corner.

### 12.3.6 Flip Vertical(V)




Reverses the image in the application area so that the top right corner of the original image is now the bottom right corner, and the top left corner of the original image is now the bottom left corner.

### 12.4 Crop(C)



**Shift+C**

Choose the **Image>Crop** command to remove the portions of an image that does not want so that the focus is on the part of the image that is left. This document instructs users on how to **Crop** an image in **ImageView**.

1. Choose the **Open Image...** command to open an image to **Crop**;
2. Choose the **Edit> Image Select** command or click the **Image Select** button  on the **Toolbar**, the cursor will change to a small cross.
3. Move the cursor over the image to the desired location, click the mouse button and hold it down to mark the first position.
4. Drag the mouse over the part of the image to be kept, a dotted rectangle appears around the selection and release the left mouse button.
5. **Optional 1:** To move the rectangle: a) Move the mouse over the selected area and when it becomes a move cursor, click and hold the left mouse button;b) Drag the selected area to the desired position.



6. **Optional 2:** To change the size of the rectangle: a) Put the mouse cursor on one of the handles that appear on the edges of the selected area; b) Click and hold the mouse button; c) Drag the box to the desired size.

**Note:** Each of the handles that appear on the edges of the box sizes the box differently.

7. To **Crop** the image, choose the **Image>Crop** command or press **Shift+C** buttons.


**Note:** If the selected area is on the video, choosing the **Image>Crop** command will capture the selected area and display it on a new image window.

### 12.5 Image Scale(S)●●●



Choose the **Image>Image Scale●●●** command to change the image to a specified size. This process actually changes spatial resolution by adding (replicating) or removing (decimating) pixels to achieve the specified dimensions.

**Width** and **Height:** When choosing the **Image Scale** command; the dialog displays the dimensions of the original image in pixels. The **Width** and the **Height** can be set on the new image by adding or removing pixels. If **Constrain Proportions** is checked, the **Width** and **Height** will stay proportionate to each other. If **Constrain Proportions** is unchecked, the **Width** and the **Height** can set independently, but this will distort the image.

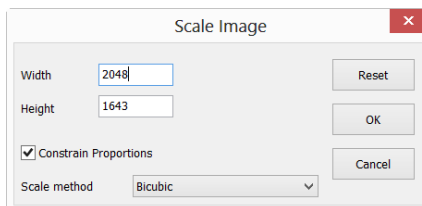

**Reset:** Reset the image **Width** and **Height** to the original ones.

**Constrain Proportions:** To maintain the current proportions of pixel **Width** and **Height**, check **Constrain Proportions**. This option automatically updates the **Width** as the **Height** is modified, and vice versa. Otherwise, uncheck the **Constrain Proportions** button.

**Scale method:** There are 3 options for the **Scale method**. They are: **Nearest Neighbor**, **Bilinear**, and **Bicubic**. The default is **Bilinear**.

### 12.6 Histogram(H)●●●



### Shift+H

A **Histogram** illustrates how pixels in an image are distributed by graphing the number of pixels at each color intensity level. The **Histogram** shows whether the image contains enough detail in the **Shadows** (shown in the left part of the **Histogram**), **Midtones** (shown in the middle), and **Highlights** (shown in the right part) in order to make a good correction.

The **Histogram** also gives a quick picture of the tonal range of the image, or the image key type. A low-key image has detail concentrated in the shadows, a high-key image has detail concentrated in the highlights, and an average-key image has detail concentrated in the **Midtones**. An image with a full tonal range has a number of pixels in all areas. Identifying the tonal range helps determine the appropriate tonal corrections.


Choose the **Image>Histogram●●●** command to open the **Histogram** dialog as shown below.

Depending on the image's color mode, choose **R**, **G** and **B**, or **Luminosity** to view a composite **Histogram** of all the channels.

If the image is **RGB** true color, choose **Luminosity** to display a **Histogram** representing the luminance or intensity values of the composite channel.



## Image

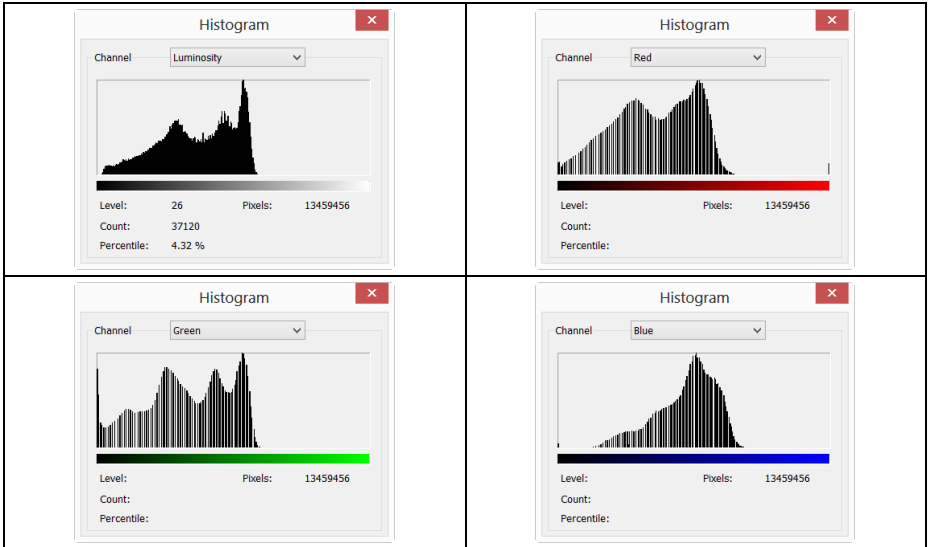

If the image is RGB true color, choose **R**, **G** and **B** to display a composite **Histogram** of the individual color channels in color.

Do one of the following:

To view information about a specific pixel value, place the mouse pointer in the **Histogram**.

To view information about a range of values, click down the left mouse button and drag it in the **Histogram** to highlight the range.

The dialog displays the following statistical information below the **Histogram**:

**Pixels**: Represents the total number of pixels used to calculate the **Histogram**.


**Level**: Displays the intensity level of the area underneath the pointer.

**Count**: Shows the total number of pixels corresponding to the intensity level underneath the pointer.

**Percentile**: Displays the cumulative number of pixels at or below the level underneath the pointer. This value is expressed as a percentage of all of the pixels in the image, from **0%** at the far left to **100%** at the far right.

## 12.7 Resolution(R)●●●

Choose the **Image>Resolution●●●** command to set the image **Resolution** to calibrate the spatial scale. By default, **ImageView** expresses spatial measurements in terms of pixels. This **Resolution** command is used to change the terms in which **ImageView** reports such measurements. This command should be run first in order to measure objects in terms of units other than pixels.

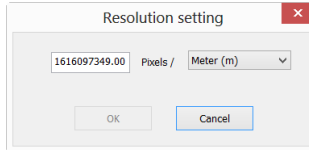

**X**: Horizontal **PPM** (**Pixels per meter**) of current **Resolution**.


**Y**: Vertical **PPM** (**Pixels per meter**) of current **Resolution**.

**Note**: The resolution in the **Y** direction need not to be filled. **ImageView** will always let it equal to the **X** direction.


After the new **Resolution** is set, all of the measurements will be calculated according to the new **Resolution**. (See more in the **Measurements and Options>Measurement●●●** menu).

## 12.8 Mosaic(O)●●●

**Mosaic** is a process that can combine the images opened into a new image. This will open the following dialog:

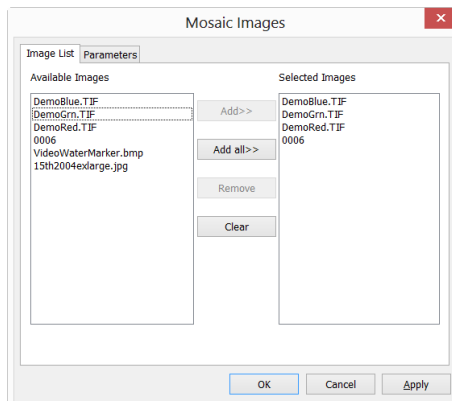

# Image

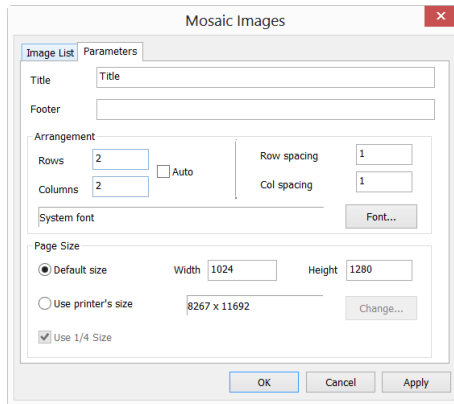

[ImgList](#) page

[Available Images](#): Images opened with [ImageView](#).

[Add>>](#): Add the opened images to the [Selected Images](#) list view

[Add All>>](#) Add all the opened images to the [Selected Images](#) list view

[Remove](#): Select the images and remove them from the [Selected Images](#) list view.

[Clear](#): Remove all the images from the [Selected Images](#) list view.

[Property](#) page


[Title](#): The title wanted

[Footer](#): The footer wanted

[Arrangement](#): The Mosaic Images distribution on the page

[PageSize](#): The page size for the Mosaic Images

If everything is set, click [OK](#) to end the Mosaic Images operations and a new image window will be displayed and the final results should be:

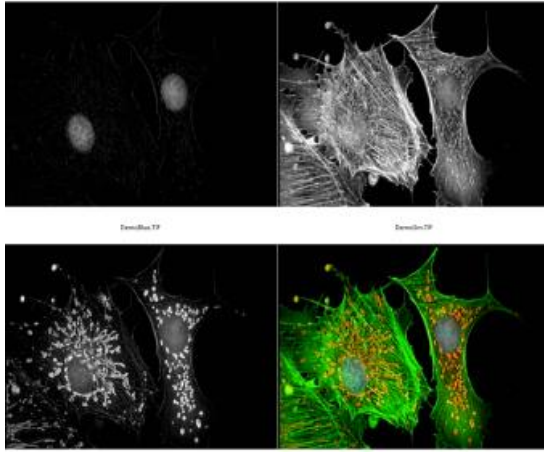

## 13 Process

### 13.1 Stitch(T)●●●



Shift+T


Image stitching or photo stitching is the process of combining multiple photographic images with overlapping fields of view to produce a segmented panorama or high-resolution image. Commonly performed through the use of computer software, most approaches to image stitching require nearly exact overlaps between images and identical exposures to produce seamless results. Some digital cameras can stitch their photos internally. Image stitching is widely used in today's world in applications such as "Image Stabilization" feature in camcorders which use frame-rate image alignment, high resolution photo mosaics in digital maps and satellite photos, medical imaging, multiple image super-resolution, video stitching and object insertion.

[ImageView](#) also integrated this function into it. It includes [Video Stitch](#), [Image Stitch](#) and [Browse Window Stitch](#).

#### 13.1.1 Video Stitch

When the video window is active, choosing the [Process>Stitch●●●](#) command will invoke the video [Stitch](#) dialog as below:

#### Capture Images

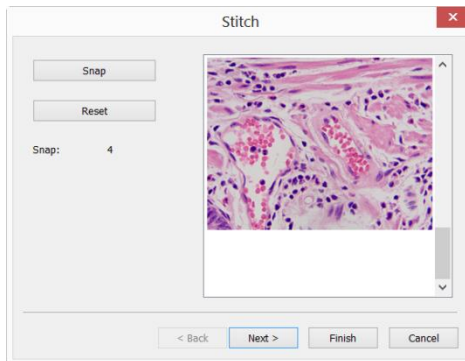

**Snap:** Click to capture image from camera. One should try to move the slide to a prop position to capture the desired images. In the moving process, the next image should have some overlaid area with the previous left or up image to ensure the success of the stitching process.

**Reset:** When an image or images is or are captured, the **Reset** button will be enabled, click **Reset** will remove it or them from the memory; It will be disabled when there is no captured image;


**Snap:** The captured images from the camera;

**Cancel:** Click to cancel the stitching process;

**Next> :** Click **Next>** will step to the next step;

**Finish:** Click **Finish** will accept the other Default setup and begin to stitch the captured images according to the above setup.

### Stitching Method

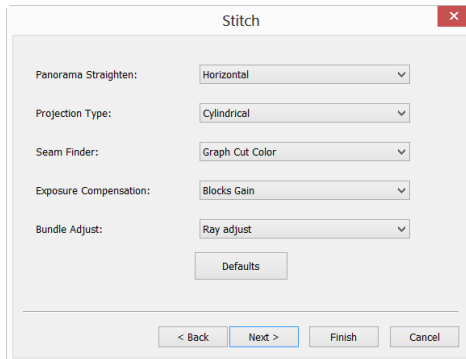

**Panorama Straighten:** The image stitching direction. It can be **Horizontal**, **Vertical** and **None**. Default is **Horizontal**;

**Projection Type:** For image segments that have been taken from the same point in space, stitched images can be arranged using one of various map projections. **ImageView** including **Plane**, **Cylindrical**, **Spherical**, **Fisheye**, **Stereographic**, **Mercator** or **Transverse Mercator** map projections. The Default is **Cylindrical**;

**Seam Finder:** Seam Finder method, **ImageView** including **None**, **Voronoi Diagram**, **Graph Cut Color** or **Graph Cut Color Grad**. Default is **Graph Cut Color**;

**Exposure Compensation:** **Exposure Compensation** is required between images to minimize exposure differences. **ImageView** including **None**, **Gain** or **Blocks Gain**

[Exposure Compensation](#) method. Default is [Blocks Gain](#);

**Bundle Adjust:** Bundle Adjustment can be defined as the problem of simultaneously refining the 3D coordinates describing the scene geometry as well as the parameters of the relative motion and the optical characteristics of the camera(s) employed to acquire the images, according to an optimality criterion involving the corresponding image projections of all points. [ImageView](#) including [Ray adjust](#) or [Reprojection error](#) adjust method. Default is [Ray adjust](#);


**<Back:** Click [<Back](#) will return to the previous setup page;

**Next> :** Click [Next>](#) will step to the next step;

**Finish:** Click [Finish](#) will accept the other Default setup and begin to stitch images according to the above setup;

**Cancel:** Click to cancel the stitching process;

### Stitching Parameter

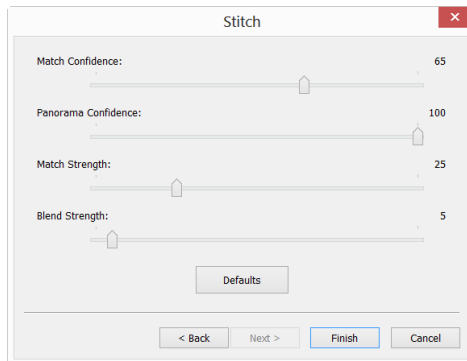

**Match Confidence:** 1~100, Default is 65;

**Panorama Confidence:** 1~100, Default is 100;

**Match Strength:** 0~100, Default is 25;

**Blend Strength:** 0~100, Defaults is 5;

**Defaults:** Click [Defaults](#) will set all the parameters to the [Default](#) ones.


## Process

---


**<Back:** Click **<Back** will return to the previous step;

**Finish:** Click **Finish** will begin to stitch images according to the above setup. After the Finish button is clicked, **ImageView** will start to stitch and a progress dialog will be shown to indicate the progress of the process.

**Cancel:** Click to cancel the stitching process;

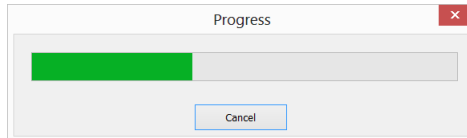

The final stitched image will be created in a new image window..

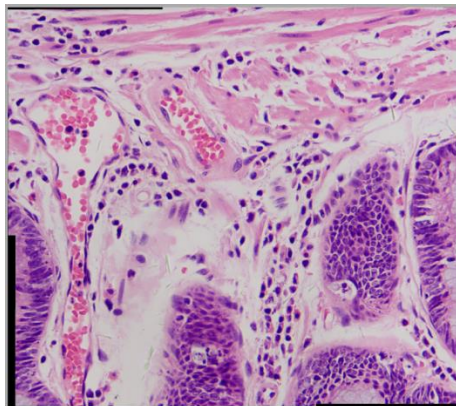


In the stitched image, there are some black areas; these are happened when there are translations among the edge images in both directions.

### **13.1.2 Image Stitch**


If images are opened in **ImageView**, for example 0001.jpg, 0002.jpg, 0003.jpg, 0004.jpg are opened as shown below:



## Process

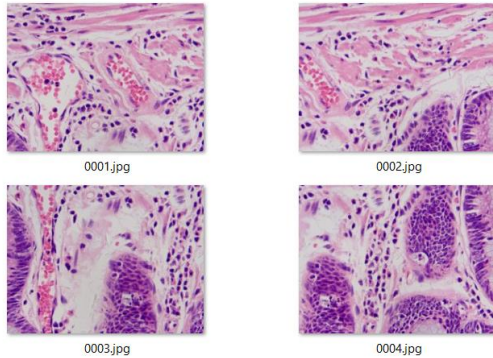

Choosing the [Process>Stitch](#) command will invoke the image [Stitch](#) dialog as shown below:

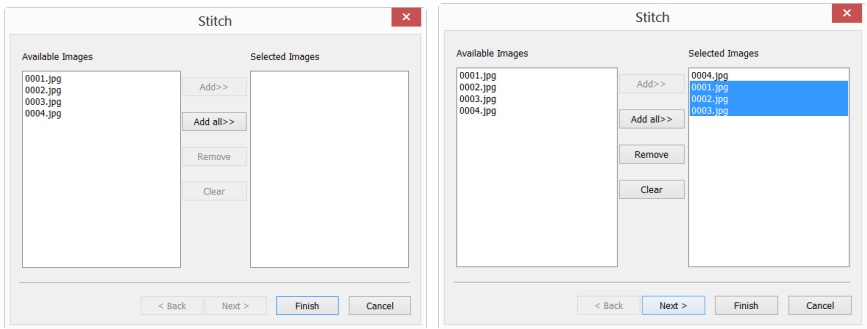

**Available Images:** The images opened by [ImageView](#); Here, 4 images are listed in the list box. One can click the image file name to select the files to be added to the [Selected Images](#);

**Selected Images:** The images selected for stitching; Using [Add>>](#) to add the [Available Images](#) to this list box;

**Add>>:** When an image or images is or are selected and highlighted in the [Available Images](#) window, the [Add>>](#) will be enabled. Click [Add>>](#) will add it or them into the [Selected Images](#) list box;

**Add All>>:** Click [Add All>>](#) will add all of the [Available Images](#) into the [Selected Images](#) list box;

**Remove:** When an image or images is or are selected and highlighted in the **Selected Images** list box, the **Remove** button will be enabled, click **Remove** will remove it or them from the **Selected Images** list box;

**Clear:** Used to clear all of the images in the **Selected Images** list box. When no image in the **Selected Images** list box, it will be disabled;


**Cancel:** Click to cancel the stitching process;

**Finish:** Click **Finish** will accept the other Default setup and begin to stitch the captured images according to the above setup;

**Next>:** Click **Next>** will step to the next step;

The other **Next>** steps are just the same as those of the **Video Stitch** process.

The final stitched image will be created in a new image window as shown below:

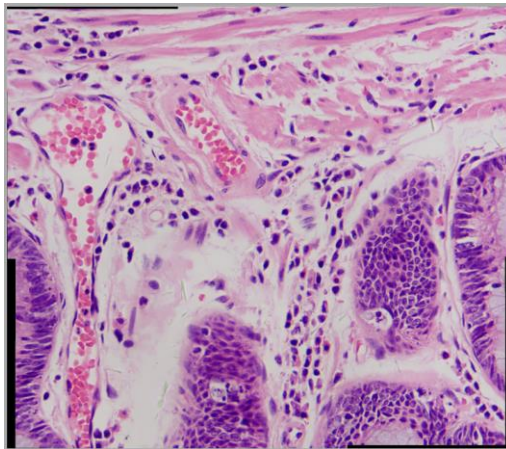

The Stitched image


In the stitched image, there are some black areas; these are happened when there are translations among the edge images in both directions.

### **13.1.3 Browse Window Stitch**


Click the **Folders Sidebar** to activate it. Double-click the right directory to show the images under the directory in the **Browse** window. Choosing the image files to be stitched and then clicking the right mouse button will display the context menu,

## Process

choose the **Stitch** submenu to start the image stitch operation (One can also choosing **Process>Stitch** to do the same operation after the files are selected in the **Browse** window)

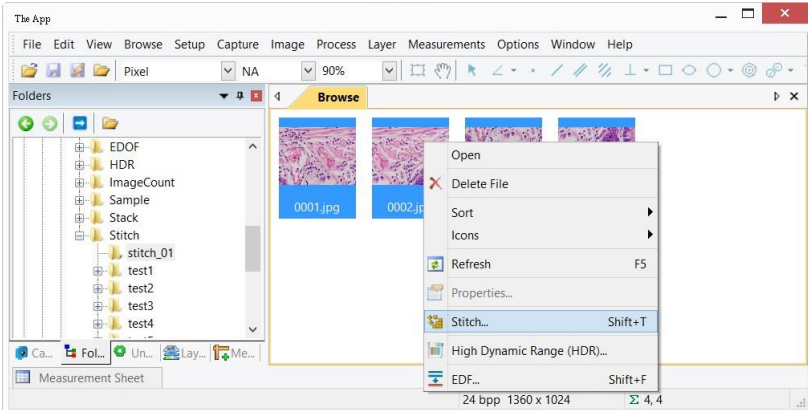


After the **Stitch** command is selected, a dialog called **Stitch** will pop up as shown below.

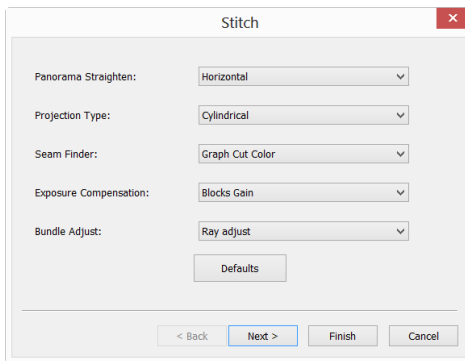

The **Stitch** dialog and the other **Next>** steps are just the same as those of **Video Stitch**. The final stitched image will look like below:

In the stitched image, there are some black areas; these are happened when there are translations among the edge images in both directions.

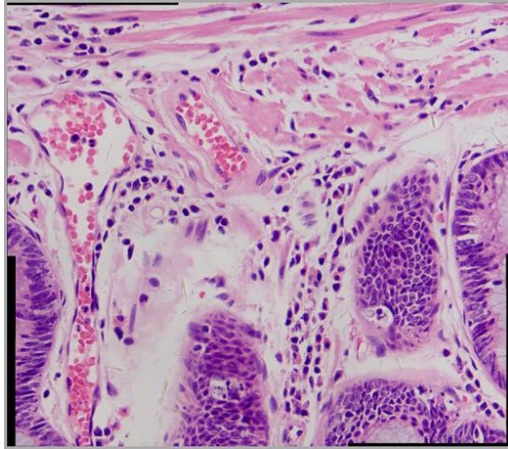

The stitched image

### 13.2 High Dynamic Range(HDR)●●●



High Dynamic Range can fuse a sequence of multi-exposure images into a high dynamic range image. The user can capture the multi-exposure images by adjust the aperture of microscope or the exposure and the gain.

ImageView support High Dynamic Range function in 2 modes, which is shown in the following part.

#### 13.2.1 Browse window high dynamic range operation

In browse window, the user can choose images to be fused directly and there is no need to open any image to save the system cost.


When the browse window is active, the user can choose low dynamic range images by **Ctrl+A** or **Ctrl+mouse left button**.

Click the right mouse button on the Browse window will invoke the context menu. Choose High Dynamic Range (or choose **Process>High Dynamic Range**), ImageView will begin to calculate according to the selected images. The high dynamic range image will be displayed in a new image window when the progress bar reaches to the end.


#### 13.2.2 Image window high dynamic range operation

## Process


When the image window is active, the user can choose images from opened window to generate high dynamic range image. This mode will lead the system to overhead when many images were opened



(1).png





(2).png



(3).png

Opened image for HDR operation

Choose [Process>High Dynamic Range](#) command to fuse captured or opened images to high dynamic range image., a dialog is called [High Dynamic Range](#) will be shown as below:

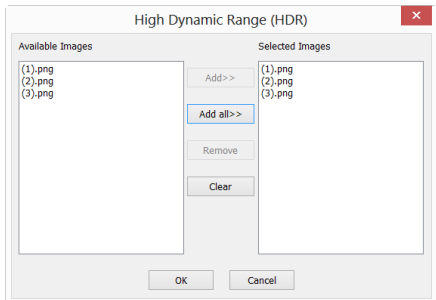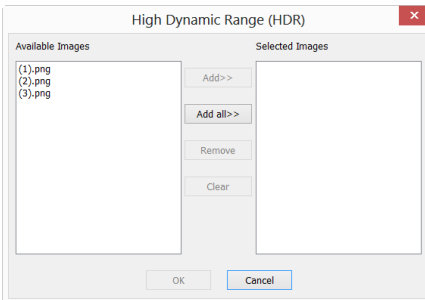

a) Available Images and b) Selected Images

We assumed that 1.jpg, 2.jpg, 3.jpg 3 images have been opened.

**Available Images:** The images opened by [ImageView](#); Here, 3 images are listed in the list box. One can click the image file name to select the files to be added to the Selected Images;

**Selected Images:** The images selected for stitching; Using [Add>>](#) to add the Available Images to this list box;

**Add>>:** When an image or images is or are selected and highlighted in the Available Images window, the Add>> will be enabled. Click Add>> will add it or them into the Selected Images list box;


**Add All>>**: Click **Add All>>** will add all of the **Available Images** into the **Selected Images** list box;

**Remove**: When an image or images is or are selected and highlighted in the **Selected Images** list box, the **Remove** button will be enabled, click **Remove** will remove it or them from the **Selected Images** list box;

**Clear**: Used to clear all of the images in the **Selected Images** list box. When no image in the **Selected Images** list box, it will be disabled;

**Cancel**: Click to cancel the stitching process;

**OK**: Click **OK** will accept the other Default setup and begin to stitch the captured images according to the above setup.

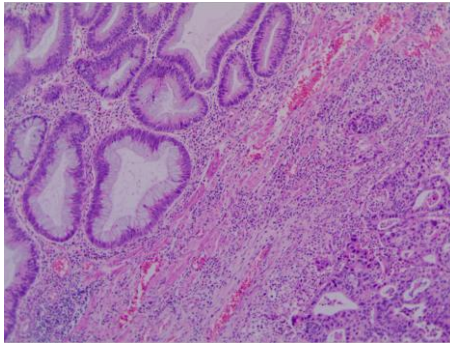

The HDR result

### 13.3 EDF●●●




**Shift+F**


#### 13.3.1 Browse Window EDF

Click the **Folders Sidebar** to activate the **Browse** Window. Double-click the directory to display the images in the **Browse** window in **Icon** mode. Choosing the image files to be fused with **Ctrl+A**(Select all files in the current directory) or **Ctrl+left mouse button** to select the image one by one and then clicking the right mouse button will display a context menu, choosing the **EDF** submenu to start the image fusion process (One can also choose **Process>EDF●●●** command to do the same operation after the image files are selected in the **Browse** window).

## Process

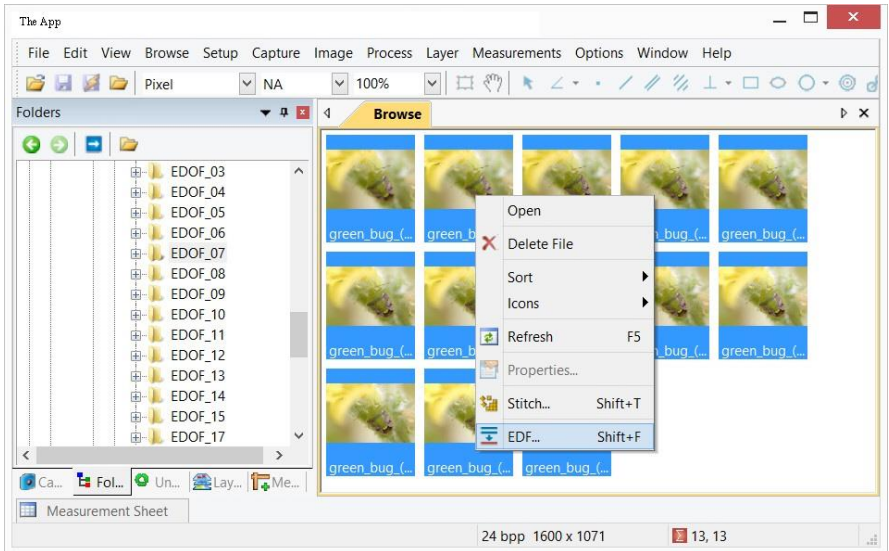

After the [Process>EDF](#) command is chosen, a dialog called [Select Method](#) is pop up as follows:

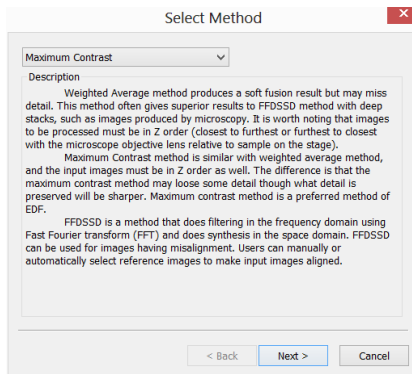

There are 3 [EDF](#) methods in [ImageView](#), they are:


[Maximum Contrast](#): [Maximum Contrast](#) method is similar with weighted average method, and the input images must be in Z order as well. The difference is that the maximum contrast method may lose some detail however the preserved details will be sharper. [Maximum Contrast](#) method is a preferred method in these 3 [EDF](#) methods.

**Weighted Average:** [Weighted Average](#) method produces a soft fusion result but may lose detail. This method often gives superior results to [FFDSSD](#) method with deep stacks, such as images produced by microscopy. It is worth noting that images to be processed must be in Z order (Capture a series images in closest to furthest or furthest to closest order);

**FFDSSD:** [FFDSSD](#) is a method that does filtering in the frequency domain using Fast Fourier transform (FFT) and does synthesis in the space domain. FFDSSD can be used for images having misalignment. Users can manually or automatically select reference images to make images aligned.

### Maximum Contrast

Choosing [Maximum Contrast](#) in the [Select Method](#) dialog will pop up an [Options](#) Dialog as follows:

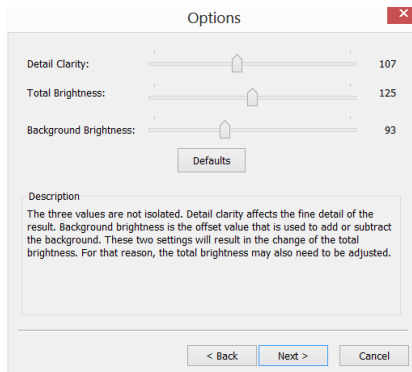

**Detail Clarity:** [Detail Clarity](#) affects the fine detail of the result. Default:107, Range: 10~240;

**Total Brightness:** [Total Brightness](#) is the overall brightness. The [Detail Clarity](#) and [Background Brightness](#) will result in the change of the [Total Brightness](#). For that reason, the [Total Brightness](#) may also need to be adjusted. Default:125, Range: 10~240;


**Background Brightness:** [Background Brightness](#) is the offset value that is used to add or subtract the background. Default: 93; Range: 10~240;



## Process

**Default:** This will set all 3 values to the Default ones;

Clicking **Next>** button will pop up an **Auto Align** dialog as follows:

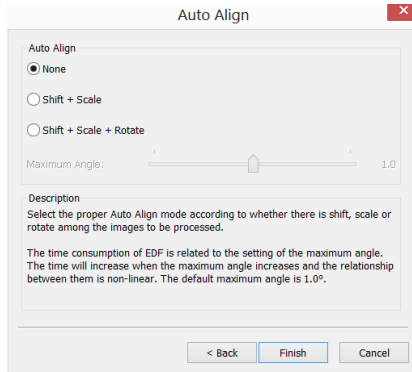

**None:** Considering no **Shift+Scale+Rotate** among the selected images in the fusion process;

**Shift+Scale:** Considering **Shift+Scale** among the selected images in the fusion process; **Rotation** is not considered in this option;

**Shift+Scale+Rotate:** Considering **Shift+Scale+Rotate** among the selected images in the fusion process; If this mode is checked, The **Maximum Angle** slide bar will be enabled;


**Maximum Angle:** The **Maximum Angle** is used to set the upper limit in **Rotate** alignment. The Default is 1 degree. Range:0.1~10;

User can select the proper **Auto Align** mode according to whether there is shift, scale or rotate among the images to be processed. The time consumption of **EDF** is related to the setting of the **Maximum Angle**. The time will increase when the **Maximum Angle** increases and the relationship between them is non-linear. The default is 1.0°;

Clicking **<Back** will return to **Option** dialog and clicking **Finish** will begin the EDF operating according to the previous setup. **ImageView** will display the **EDF(Extended Depth of Focus)** progress bar as follow:

## Process

---

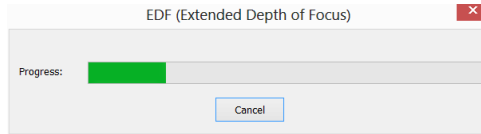

The final EDF result is shown below:



### Weighted Average

The setups of the [Weight Average](#) are the same as those of the [Maximum Contrast](#). About the setup details, please refer to [Maximum Contrast](#).

### FFDSSD


Choosing [FFDSSD](#) in the [Select Method](#) dialog will pop up a [FFDSSD Options](#) dialog as below:

[Determine the reference image automatically](#): Before [EDF](#), [FFDSSD](#) will evaluate all the images to determine the reference image for feature matching. After the reference image is determined, [FFDSSD](#) will perform feature matching between the reference image and the other images to find the alignment parameters


If the [Determine the reference image automatically](#) is unchecked, [ImageView](#) will take the first image as reference image in the alignment operation.

## Process

---

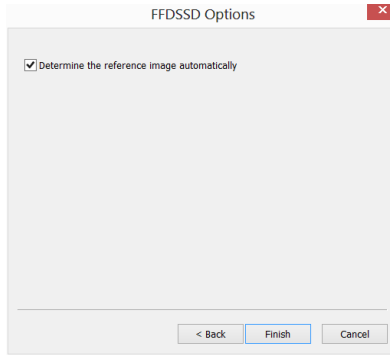

Clicking **Finish** button will begin the **EDF**, an **EDF (Extended Depth of Focus)** progress bar dialog will display as follows:

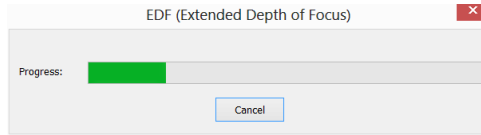

The final **EDF** result is shown below:




### 13.3.2 Image Window EDF

Similar to the **Browse** window **EDF**, **Image** window **EDF** is also a very useful tool to generate a clear image by combining a sequence of previously captured or opened multi-focus images. Choosing the **Process>EDF•••** command, the following dialog will be brought up (assume 01.jpg 02.jpg ••• 15.jpg are already opened in **ImageView**):

## Process

---

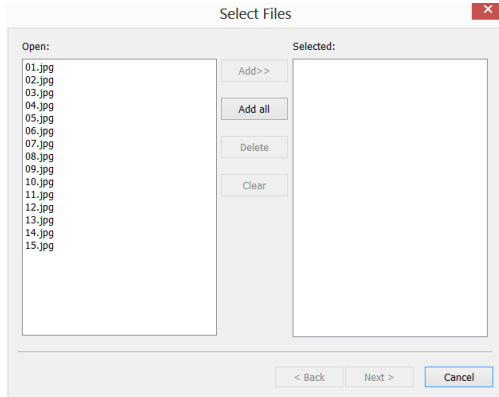

Clicking on the image file name in the **Open** combobox will highlight the image, and then the **Add>>** button is enabled (Click on the selected images will deselect them). Click the **Add>>** button, the highlighted images will be added into the **Selected** list box, which will be fused later.


Clicking the **Add all** button will add all images in the **Open** combobox into the **Selected** list box.

If images in the **Selected** combobox are highlighted, the **Delete** button will be enabled. Click the **Delete** button, the highlighted images in the **Selected** combobox will be removed.

Clicking the **Clear** button will remove all the images in the **Selected** list box, including the unselected ones. The button will be disabled if there is no image in the **Selected** combobox.

When the desired images are all selected (If more than 2 images are added in the **Selected** List box, the **Next>** button will be enabled), clicking on the **Next>** button will start the other **EDF** setup as those of the **Browse** window **EDF**. After all of the setup is finished, **ImageView** will display the **EDF(Extended Depth of Focus)** progress bar as follows:


## Process

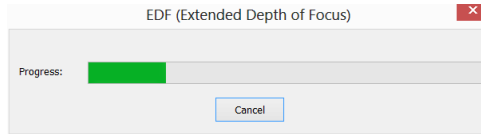

The final EDF result is shown below:




**NOTE:** Images used for fusing must be the same size; otherwise there will be a prompt when adding different sizes of image to perform the EDF operation. The prompt dialog indicates which image is not the same size with the others.

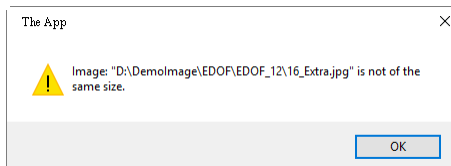

### 13.3.3 Video Window EDF




Make sure that the [ImageView](#) package and the camera are correctly installed. Turn on the microscope's light.

1. Run [ImageView](#) and start the camera;
2. Choosing the [Process>EDF...](#) command or clicking  on the toolbar will bring up a dialog called "[Capture Image](#)";
3. Use the microscope [coarse](#) or [fine](#) focus knobs to move the sample stage up and down, in order to find the positions where the clearest regions of the whole sample

can be seen on the [Video](#) window;

4. Click the [Capture](#) button to capture an image into the image list which will be used for the [EDF](#) operation.

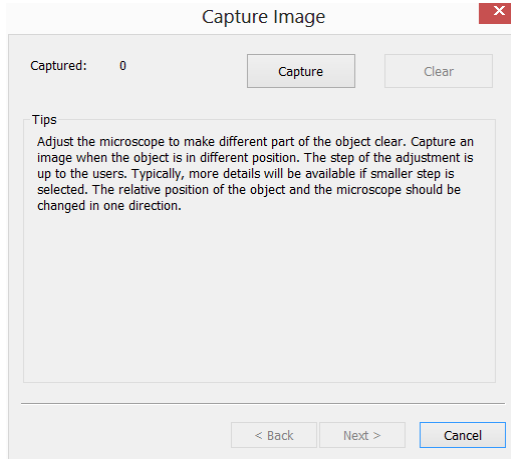

5. Unless there is 1 captured image, the [Clear](#) buttons will not be enabled. Unless there are more than 2 captured images, the [Next>](#) buttons will not be enabled. If the captured images are not satisfactory, click the [Clear](#) button to clear the captured image(s) and capture new image(s).

6. If more than 2 images are captured, Clicking [Cancel](#) will end the [Capture Image](#) and return to the [Video](#) window. If the [Next>](#) button is clicked, [ImageView](#) will pop up a dialog called [Selected Method](#) to begin the [EDF](#) configuration process. About the configuration detail, please check [Browse Window EDF](#) in this section.



The final fused image will be displayed in a new active image window and its title bar will be associated with a digit assigned by [ImageView](#).

**Note:** a). Use the [coarse](#) and [fine](#) focus knobs to move the sample stage up and down; b). Clicking the [Capture](#) button will capture the current image into the image fusion list; c). Repeating steps 1-4 until there are enough images; d). Clicking the [Fusion](#) button will start image fusion. Waiting for some time and a fantastic fusion result will be displayed in a new image window;

### 13.4 Deinterlace(A)

When interlaced cameras is used to take the images, a complete images is divided into 2, 3 or more fields. Since different fields are exposed and output at different time, there is no problem for a still object. But you will see an image with interlaced content when the object is moving. Deinterlacing algorithm is used to resolve this problem. This function could find the difference between different fields automatically, correct the location difference as much as possible and deinterlace the image. But vertical resolution will be lost to some extent and there will be some small shift.

### 13.5 Color Composite(C)●●●




Use the [Color Composite](#) dialog box to create and configure color composites using black and white source images. You can access the [Color Composite](#) dialog box through the [Color Composite](#) menu item from the [Process](#) menu.

You can combine gray-scale images into a color composite. Any group of gray-scale images that are of the same size can be mixed in a color composite. Images of 8-, 12-, 16-bit integer or floating point format are combined into a 24-bit color composite. Each input channel will have individual LUT adjustments, as well as a registration offset to line it up with the rest of the images.

You can also combine individual channels from a single image. Each channel will be listed separately, as shown here:

## Process

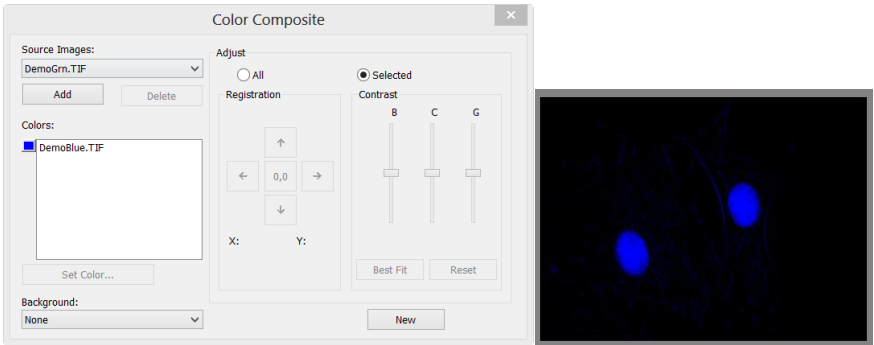


**Source Images:** The **Source Images** combo box displays the images available for color mixing. The **Source Image** list is initially filled with a list of the gray scale images that are currently open. The size of the color composite is determined by the first input image selected. Once this is entered, the list is filtered to contain only images of the same size as the initial selection.

**Add:** Click the **Add** button to add an image to the mix. You will be prompted for the color to be assigned to that image from the **Set Color** dialog.


**Delete:** Use this button to delete the selected image from the list.

**Colors:** The **Colors** combobox displays the images selected for color mixing.

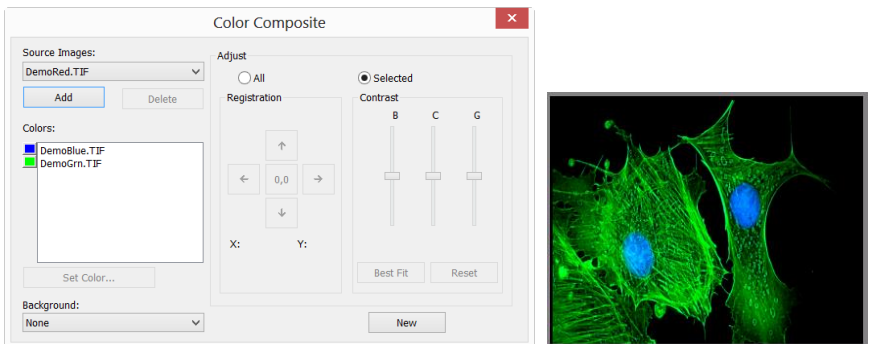



## Process

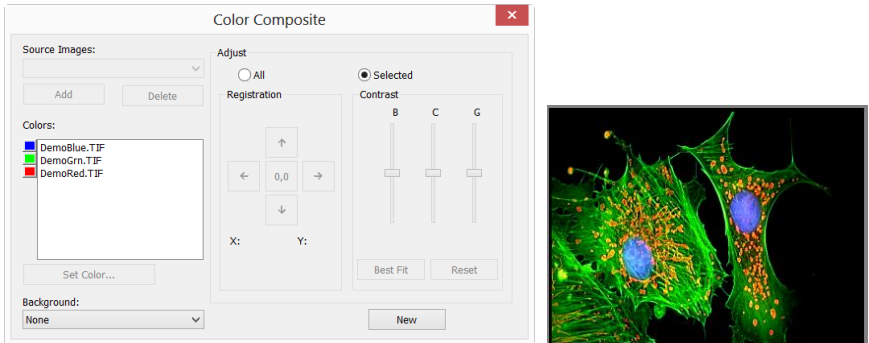


To change the color within the list box, double-click to select the image name (the [Select Color](#) dialog box appears) or highlight the name and click the [Set Color](#) button.

To delete colors/images from the [Colors](#) list box, first click on the color/image to highlight it then press the [Delete](#) button within the [Color Composite](#) dialog box.

[Color Bar](#): The picture item box on the left side of the [Colors](#) list indicates the color associated with each image in the composite. The [Color Bar](#) will scroll with the contents of the [Colors](#) list box.

[Set Color](#): This option determines the [Color](#) value used for the selected channel in the final image display. Clicking on the [Set Color](#) button brings up the [Select Color](#) dialog box.

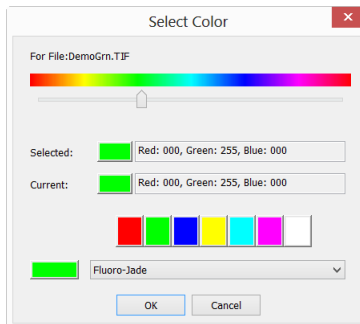

Directly select a color by:

1) Dragging the [Color Value Slider](#) to the desired color on the [Color Bar](#) (range of 0 to 359°): or

2) Clicking the appropriate **Color** button on the **Color Palette**. The **Color Bar** represents **Color** degrees in the standard color wheel representation, and the **Color Palette** contains a subset of possible **Colors** (pure red, green, blue, cyan, magenta, and white): or

3) Select a dye in the dye list, and click the **Select Dye** button.

**Note:** You can navigate through the **Select Color** dialog box by using the **<Tab>** and **<Shift + Tab>** keys to cycle through the items in the dialog box.

**Intensity** is determined by the image the **Color** is applied to, and **saturation** will always be 100%.

The only exception to this is the "white" **Color**, which has by definition a saturation of 0%. Selecting a value greater than or equal to 360 (dragging the **Color Value** slider over to the far right) is a choice of white, which results in a non-tinted (gray) image.

The elements of the **Select Color** dialog box are:

**Color Bar:** The **Color Bar** shows a rainbow displaying the **Colors** underneath the appropriate point of the **Color Value** slider.

**Note:**

If **Color Value Slider** is the selected (highlighted) selected control, then you can also control the slider with keyboard strokes:

Use the left/right arrow **<->** or **<->** keys to move the slider incrementally.

Press the **<Page Up>** and **<Page Down>** to move the slider in "chunk" sections along the **Color Bar**.

Use the **<Home>** and **<End>** keys to move the slider to the beginning and end of the **Color Bar**.

**Selected:** This color block displays the new **Color** selected by the **Color Value** slider bar or the **Color Palette**.

**Selected Color:** The **Selected Color** text field displays the corresponding numeric **Color** value of the **Selected** color block described above. The **Selected Color** value is

expressed as an **HSV** color, with the red value first, followed by the green and blue values. If the color corresponds to a dye color, the dye name will be displayed. If the dye color corresponds to a color palette color, the name of the color will also be displayed.

**Current:** The **Current** color block displays the starting **Color** of the channel.

**Color Palette:** The **Color Palette** provides an alternate method of selecting a **Color**. Clicking on an item in the **Color Palette** will set the **Color Value** slider to the correct value and update the displays in both the **Selected** color block and **Selected Color** text field.

For example, clicking on the white button on the **Color Palette** will set the **Color Value** slider to the right, change the **Selected** color block to white, and cause the **Selected Color** text box to display "White".

**Adjust:** The controls in this section are used to adjust the color composite contribution from each image, or for the color composite preview itself. You can adjust the input image that is currently selected in the **Colors** list by clicking the selected button. When you want to adjust the color composite preview, or you want no image is selected in the **Colors** list, use the **All** button.

**Registration:** **Registration** allows you to correct for mis-registrations of images caused by filter-induced optical shifts. Use the directional keys to shift the selected image in the x- and/or y- direction, with respect to the rest of the input images. One click moves that channel one pixel in the direction indicated. Blank areas are filled with black. The key labeled "0,0" will re-center the selected image.

The registration shift for the selected channel or the overall image is displayed in the static text box below the directional keys.

**Contrast:** Use the **BCG sliders** along with the **Best Fit** and **Reset** buttons to adjust the contrast of the selected image or the composite.

**BCG sliders:** The **Brightness**, **Contrast**, and **Gamma** sliders are similar to the **Contrast Enhancement** feature in **ImageView**. You can also adjust each channel individually or collectively by using the **Selected** or **All** radio buttons (to the left of the **BCG** sliders in the **Adjust** group box).

**Best Fit:** Click this button to perform a **Best-Fit** contrast stretch on the selected input, automatically setting the Brightness and **Contrast** settings accordingly (**Gamma** will be reset to 50.). This method is identical to the **Best Fit** contrast adjustment under the standard **Contrast Enhancement** feature of **ImageView**. **Best Fit** is useful for first pass adjustments.

**Reset:** Pressing the **Reset** button automatically resets the **BCG** settings. If the **Adjust** radio button is set on **All**, the **BCG** settings for the overall color image will be reset.

**Frame:** Use the frame slider to adjust the frame of the selected image that is used for the preview, or the active frame of the composite. (Please see the discussion of **Color Composite** and **Image Sequences** that follows this section.)

**Background:** Select one of the available images to be the background color in this combo box. The rest of the image planes are subtracted from the background image — effectively punching “holes” into it and allowing the foreground colors to show without mixing with the background. This is most effective where the background covers large areas and the other images have smaller objects within the background objects.

**Background** allows the other inputs to be displayed “in front of” the background inputs, minimizing color mixing. For example, **ImageView** can display a red dot on a blue background without turning the dot to magenta.

Selecting **None** causes all images to be equally mixed.

**New:** Click on the **New** button to discard the current color composite image, and start over.

The **Source Images** combo box will reset to include all gray scale images (including floating point images). Selecting an image from the list will create a new composite the same size as the initial selection. As mentioned previously, the source images list will be filtered to contain only images of the same size as the initial selection.

### **13.6 Segmentation & Count●●●**

Choose the **Process>Segmentation & Count** command to realize the segmentation and count of the interested image. The arrangement of **Segmentation & Count** is very special and some explanations are needed here to clarify it in details:

1. The function provides users with five methods which are [Watershed\(W\)](#), [OTSU Dark](#), [OTSU Bright](#), [RGB Histogram](#), [HSV Histogram](#) and [Color Cube](#). Users can select any one of those 5 methods, but after selecting any one of them, the others will be disabled.
2. After segmentation, there may exist adhesions. Then what we should do is segment connected object manually by choosing the [Split Objects](#) function.
3. When the users get the expected results, they can choose the [Counting Results](#) menu and get the statistics and analysis results.

According to the counting result, you can go back from step 2 or 3 to step 1 or 2 to repeat segmentation or split objects operation.

**Note:** If the users choose [None](#) in the [Label](#) button at the [Count Options](#) dialog, then regardless of the type of [Method](#) set, there is no [Label](#) for [Index](#), [Area](#) or [Perimeter](#) on the image. But the [None](#), [Circle](#) and [Ellipse](#) will show the segmentation results. That's why [ImageView](#) name the menu as [Segmentation & Count](#). That is, this function can achieve either the image [Segmentation](#) or [Count](#). In this regard, please refer to the [Process>Segmentation & Count > Watershed\(W\)](#) in the [Count Options](#) dialog.


### 13.6.1 Watershed(W) ●●●

[Watershed](#) segmentation method is a mathematical morphology segmentation method, which based on topological theory. The basic idea is taking the image as a topological geomorphology on geodesy, and each image pixel gray value indicates the altitude, boundaries of each local minimum value and its impact area called catchment basins and the formation of watershed catchment basins. So the formation of the watershed concept can be illustrated by simulating the immersion process. In each local minimum value of the surface, piercing a hole, then the entire model slowly immersed in water, with the immersion of the deepening impact of the domain of each local minima slowly expands outward in two catchments basin at the confluence build dams that form the watershed.

[Watershed](#) is suitable for relatively simple background target object or target object with a relatively large difference between the background images instead of the more complex application.

## Process

Choose **Process>Segmentation & Count > Watershed(W)...**, there will pop up the following dialog: (**Note:** **Segmentation & Count** function only works for 24 bits, otherwise all the sub-menu items will be disabled. Users can change the **Color Bits** to 24 bits by choosing **Image>Mode>Color Quantize...**)

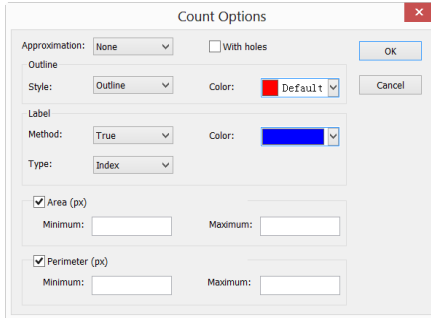

**Approximation:** **Approximation** including 3 options: 1)**None**: drawn the actual outline of the segmented object; 2)**Circle**: The actual outline fitting into a perfect circle, users can get fit **Radius** of each object in the **Count Result** dialog; 3)**Ellipse**: The actual outline fitting into a ellipse, users can get fit **Axis** of each object in the **Count Result** dialog;

**With Holes:** When checking **With Holes** function, the segmented object's **Outline** will be marked with **Color**. Meanwhile the holes are also marked with **Color** and its parameters will be output in the image (**Hole** is defined as the target grayscale or the color close to the background pixels). The left figure below is the segmentation result without checking **With Holes**; the right below is on the contrary. **With Holes** option is usually used to get hole parameters;



**Outline: Style:** Including 3 options: 1)**Outline**: objects are marked by outline, the color can be user-defined; 2)**Filled**: the segmented objects will be filled with custom colors; 3)**None**: no marked outline for the segmented object;

**Color:** Custom colors used to mark the **Style**;

**Label: Method:** Including 3 options: 1) **XOR**: with the current pixel's **XOR** color to mark the current object segmentation; 2) **True**: marked with the specified **Color**; 3) **False**: no mark for the objects;

**Note:** If users choose **False** in the **Label** group box, then regardless of the type of **Method**, there is no display for **Index**, **Area** or **Perimeter**. But the **None**, **Circle** and **Ellipse** will be displayed on the segmented image. That's why **ImageView** call it **Segmentation & Count**;

**Color:** Custom **Color** used to represent the color of **Label**. When selecting **XOR** in the **Method**, the **Color** selection will be disabled, but the **ImageView** will automatically mark the segmented image with the current pixel's **XOR** color;

**Type:** Including 3 options: 1) **Index**: use numbers to mark the segmented object. 2) **Area**: the object area is marked by outline area size. 3) **Perimeter**: the object perimeter is marked by the outline perimeter;

**Area:**

**Minimum:** determine the lower limit of the area. that is, if the object area is less than the lower limit, it will not be included;


**Maximum:** determine the upper limit of the area. that is, if the object area is greater than the upper limit, it will not be included;

**Perimeter:**

**Minimum:** determine the lower limit of the perimeter. that is, if the object perimeter is less than the lower limit, it will not be included;

**Maximum:** determine the upper limit of the perimeter. that is, if the object perimeter is greater than the upper limit, it will not be included;


The figure below shows image **Segmentation & Count** results with watershed method with setting in **Count Option** dialog.

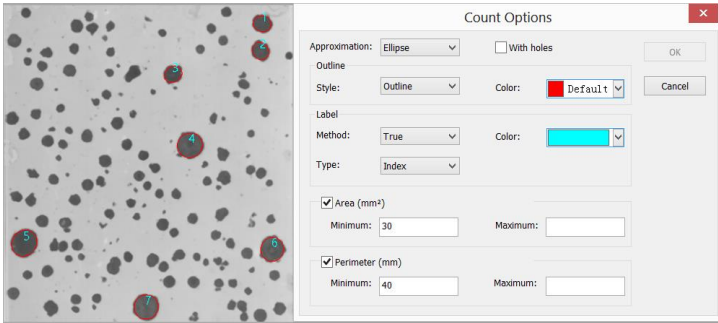

### 13.6.2 OTSU Dark(D)●●●

OTSU is proposed in 1979 by Japanese scholars, which is a method to determine the threshold of an adaptive, also known as Otsu method, referred to as OTSU. It is based on the gradation characteristic of the image, and divided the image into the background and the target. The bigger the OTSU is between background and the target, the larger difference between the two parts images. The wrong part of the the background or the wrong part of the target will lead to smaller differences between the two parts. Therefore, the maximum OTSU means the minimum probability of misclassification.

OTSU Dark segmentation method means segment the dark object from the bright background using OTSU algorithm. Its [Count Options](#) dialog is exactly the same with the [Watershed Count Options](#). Below are bright background with dark object (bottom left) and its segmentation result (bottom right) for reference:

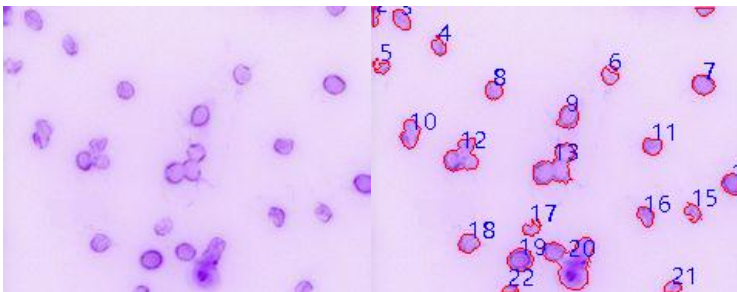


### 13.6.3 OTSU Bright (B) ●●●

OTSU Bright segmentation method means segment the bright object from the dark background using OTSU algorithm. Its [Count Options](#) dialog is exactly the same with




the [Watershed Count Options](#). Below are dark background with bright object (bottom left) and its segmentation result (bottom right) for reference:

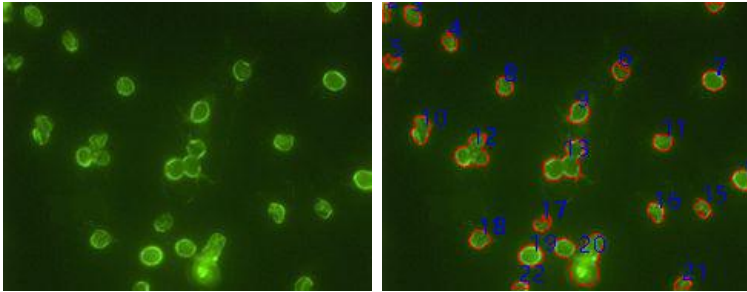

### 13.6.4 RGB Histogram ●●●

[RGB Histogram](#) segmentation is based on image histogram where image pixels between a specified histogram upper and lower range will be color processed. The segmented area can be adjusted by mouse to drag two vertical lines in histogram, or by inputting precise value in [RGB](#) upper and lower edit box directly and clicking “Enter” to make it effective. The [Color](#) representing the segmentation area can be customized by system palette. For a 24-bit true color image, segmentation can be realized by R, G, B channels respectively.

Choose [Process>Segmentation & Count>RGB Histogram●●●](#) shows [Histogram](#) dialog, each function is specified as below:

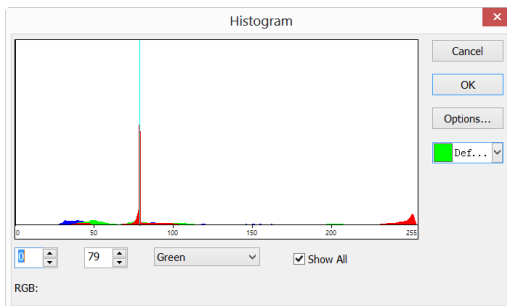

: [Left Value](#) in the currently selected region of histogram segmentation, corresponding to [Left Vertical Line](#) position in histogram. Users can segment the pixels bigger than the [Left value](#) by inputting a value in this edit box or dragging the [Left Vertical Line](#) in histogram. When input a [Left Value](#) in this edit box, users should

click enter to make the value effective. Meanwhile, the [Left Vertical Line](#) will move to the place the [Left Value](#) represents. [Left Value](#) range: 0~current [Right Value](#). The current [Left Value](#) is 0;


: [Right Value](#) in the currently selected region of histogram segmentation, corresponding to [Right Vertical Line](#) position in histogram. Users can segment the pixels, bigger than the [Left Value](#) and smaller than [Right Value](#), by inputting a value in this edit box or dragging the [Right Vertical Line](#) in histogram. When input a value in this edit box, users should click enter to make the value effective. Meanwhile, the [Right Vertical Line](#) will move to the place the [Right Value](#) represents. Range: The current [Left Value](#) ~255;

: A histogram channel of the currently [RGB](#) histogram. It can be [R](#) histogram, [G](#) histogram or [B](#) histogram;

Show All : Show all channel [RGB](#) histogram. When uncheck [Show All](#), only a selected histogram channel will be shown;

: Used to identify the [Color](#) of the segmented pixels; The default is green;


: When users click [Options...](#) button, a [Count Options](#) dialog pops up as below. The setting of [Count Options](#) dialog is the same as that of [Watershed's Count Options](#) dialog, details can be referred to [Process>Segmentation & Count>Watershed\(W\) ...](#);

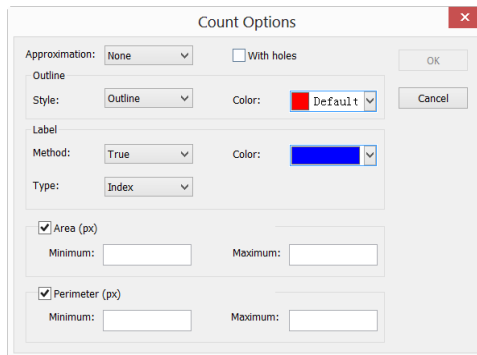

Example of [RGB Histogram](#) is as follows:

## Process

1. Open an image and then choose **Process>Segmentation & Counting>RGB Histogram...** menu, a **Histogram** dialog shows as below. When the mouse moves in the image area, the cursor will be displayed as **Color Picker Cursor**;

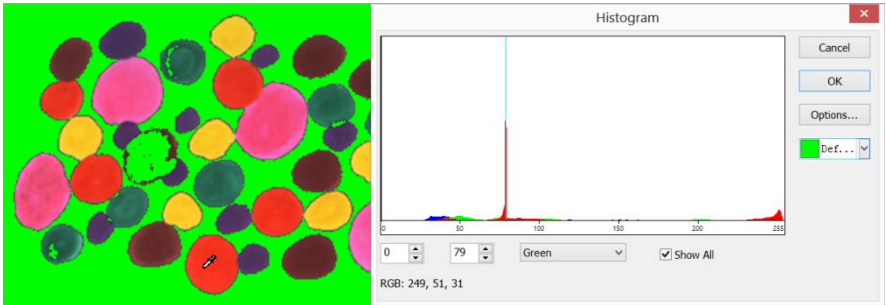

2. Move **Color Picker Cursor** to any pixel of the image, shown as above, **RGB** value of the current pixel will be displayed in the bottom Histogram window. Here **R** is 249, **G** is 51, **B** is 31, showing the **RGB** value of the ideal segmentation area, record the three values.


3. Move the mouse to the background area, the **RGB** value of **Color Picker Cursor** is 79, 79, 79. In order to accurately segment out the target, users can set **RGB** values of the segmented pixels in the initial interval, and those of background out of the initial interval. For example, the **RGB** values can be set to the initial interval as follows:

**R** is set to the initial interval: 200~255;


**G** is set to the initial interval: 0~60;

**B** is set to the initial interval: 0 ~ 60;


When setting completed, the segmentation effect is shown as below:

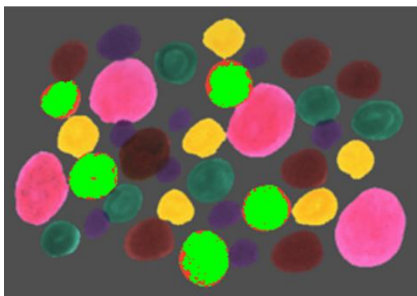

4. Move again the **Color Picker Cursor** to any other unshaded pixels, then the **RGB** value shown in left bottom of histogram is 237, 70, 45 as below:

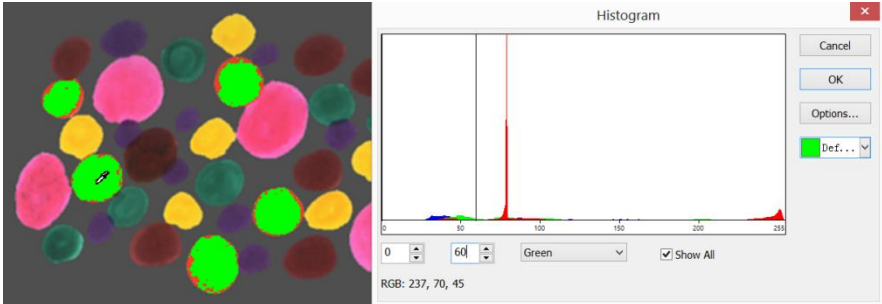

It's easily found that here **G** channel, defined 60, is too small to get the pixel segmented. Then initial interval for **G** channel can be adjusted from 0~60 to 0~80 to segment the pixels nearby. (**Note:** If the background pixels of a single channel is within the initial interval, no segmentation change will take place. Only all three channels of the background pixels are within the initial intervals can the pixels be segmented) The segmentation effect by readjusting **G** initial interval is shown as below:

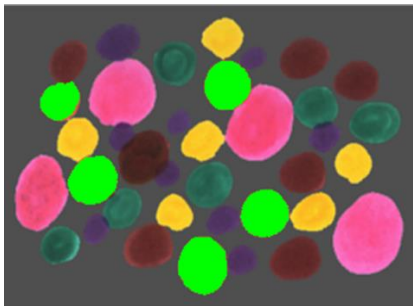


5. Repeat step 4 and readjust initial interval of each **RGB** channel to achieve perfect segmentation.

### 13.6.5 HSV Histogram●●●

**HSV Histogram** segmentation is based on image histogram where image pixels between a specified histogram upper and lower range will be color processed. The segmented area can be adjusted by mouse to drag two vertical lines in histogram, or by inputting precise value in **HSV** upper and lower edit box directly and clicking

“Enter” to make it effective. The **Color** representing the segmentation area can be customized by system palette. For a 24 bits true color image, segmentation can be realized by **H**, **S**, **V** channels respectively.

Choose **Process>Segmentation & Count>HSV Histogram** shows **Histogram** dialog, each function is specified as below:

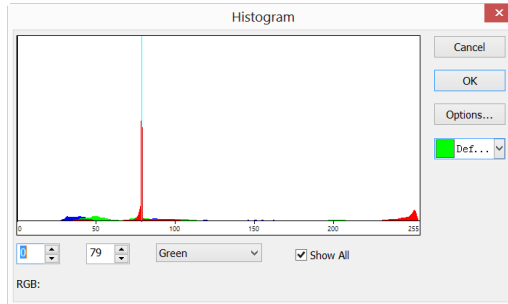


: **Left Value** in the currently selected region of histogram segmentation, corresponding to **Left Vertical Line** position in histogram. Users can segment the pixels bigger than the **Left value** by inputting a value in this edit box or dragging the **Left Vertical Line** in histogram. When input a **Left Value** in this edit box, users should click enter to make the value effective. Meanwhile, the **Left Vertical Line** will move to the place the **Left Value** represents. **Left Value** range: 0~current **Right Value**. The current **Left Value** is 0;


: **Right Value** in the currently selected region of histogram segmentation, corresponding to **Right Vertical Line** position in histogram. Users can segment the pixels, bigger than the **Left Value** and smaller than **Right Value**, by inputting a value in this edit box or dragging the **Right Vertical Line** in histogram. When input a value in this edit box, users should click enter to make the value effective. Meanwhile, the **Right Vertical Line** will move to the place the **Right Value** represents. **Right Value** range: current **Left Value** ~255. The current **Right Value** is 79;


: A histogram channel of the currently **HSV** histogram. It can be **H** histogram, **S** histogram or **V** histogram;

**Show All** : Show all channel **HSV** histogram. When uncheck **Show All**, only a selected histogram channel will be shown;

## Process


: Used to identify the **Color** of the segmented pixels; The default is green;

: When users click **Options...** button, a **Count Options** dialog pops up as below. The setting of **Count Options** dialog is the same as that of **Watershed's Count Options** dialog, details can be referred to **Process>Segmentation & Count>Watershed(W)...**;

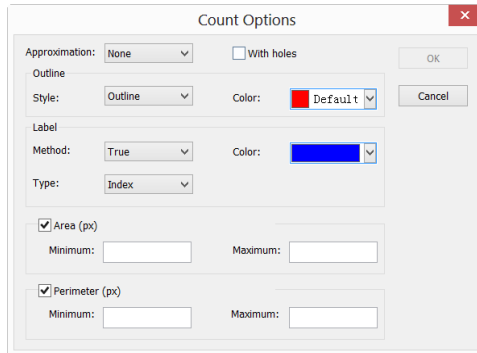

Example of **HSV Histogram** is as follows:

1. **Open** an image and then choose **Process>Segmentation & Counting>HSV Histogram...** menu, a **Histogram** dialog shows as below. When the mouse moves in the image area, the cursor will be displayed as **Color Picker Cursor**;

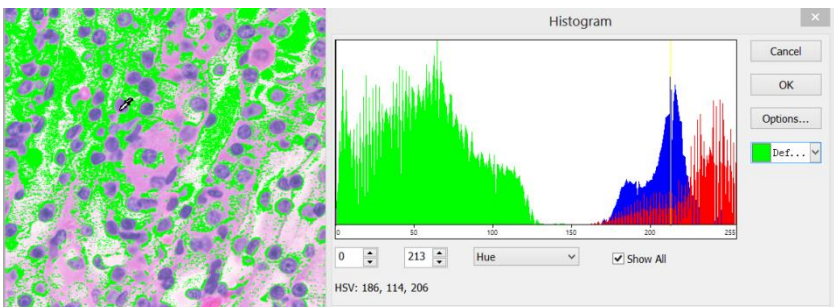

2. Move **Color Picker Cursor** to any pixel of the image, shown as above, **HSV** value of the current pixel will be displayed in the bottom Histogram window. Here **H** is 186, **S** is 114. **V** is 206, showing the **HSV** value of the ideal segmentation area, record the three values.

## Process


3. Move the mouse to the background area, the HSV value of Color Picker Cursor is 214, 87, 228. In order to accurately segment out the target, users can set HSV values of the segmented pixels in the initial interval, and those of background out of the initial interval. For example, the HSV values can be set to the initial interval as follows:

H is set to the initial interval: 60~200;


S is set to the initial interval: 90~130;

V is set to the initial interval: 0~210;

When setting completed, the segmentation effect is shown as below:

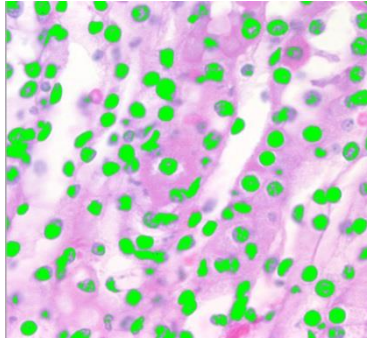


4. Move again the Color Picker Cursor to any other unshaded pixels, then the HSV value shown in left bottom of histogram is 194, 79, 212 as below:

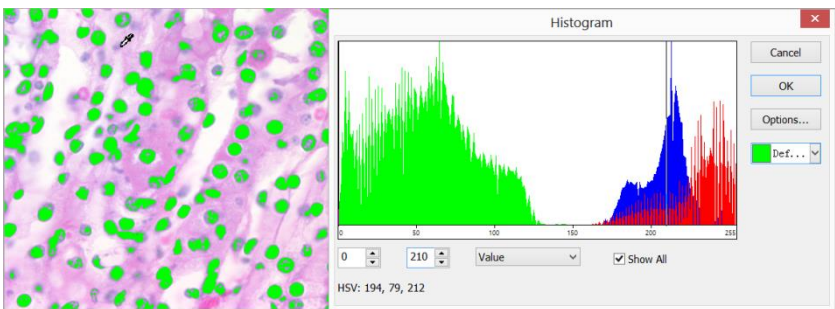

It's easily found that here S channel, defined 90~130, its lower limit is too big to get the pixel segmented. Then initial interval for S channel can be adjusted from 90~130 to 60~130 to segment the pixels nearby. (Note: If the background pixels of a single channel is within the initial interval, no segmentation change will take place. Only all


three channels of the background pixels are within the initial intervals can the pixels be segmented) The segmentation effect by readjusting **S** initial interval is shown as below:

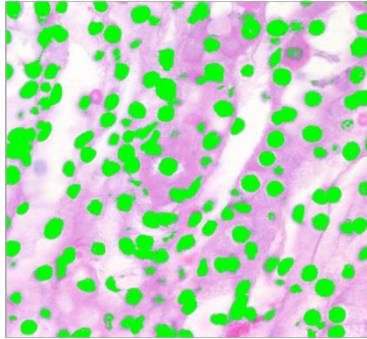

5.Repeat step 4 and readjust initial interval of each **HSV** channel to achieve perfect segmentation.

### 13.6.6 Color Cubic(C)●●●

Choose **Process>Segmentation & Count>Color Cube●●●**, a dialog called **Color** will pop up as below;

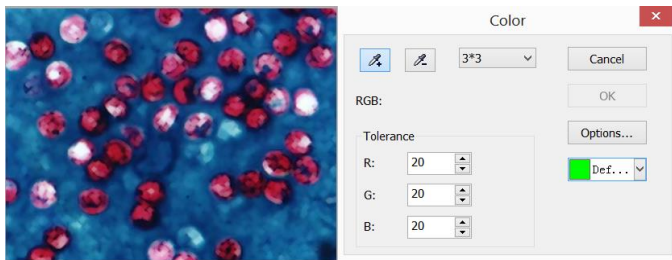



At this moment, the **Colorizing Pipette** (Default) is checked by default. Click the image will set the average color value in the masked area as **Basic Value**. **ImageView** will segment the image by choosing the pixel within **Basic Value±Tolerance** color range and mark it with current selected **Color**. By clicking the target pixel repeatedly, **ImageView** can continuously add new pixels within the **Basic Value±Tolerance** color range into the target and thus acquiring continuous segmentation coloring.


When some undesirable pixels have been added into the segmentation data, the



**De-Colorizing Pipette** can be used to wipe off the undesirable pixels. This operation process is the same as **Colorizing Pipette**, that is, to set the average color value of the clicked-pixel's **Mask Area** as **Basic Value** and wipe off the segmentation data, which is within the **Basic Value±Tolerance** color range.


 **Colorizing Pipette**: Collect average color value of the clicked-pixel's **Mask Area** as **Basic Value** and add pixels which are within **Basic Value±Tolerance** color range into the segmentation data;


 **De-Colorizing Pipette**: Collect average color value of the clicked-pixel's **Mask Area** as **Basic Value** and wipe off the segmentation data, which is within the **Basic Value±Tolerance** color range;

 **Mask Area**: When **Colorizing Pipette** or **De-Colorizing Pipette** is used to click the image, a **Mask Area** is also needed to calculate the average color value of the clicked pixel. The **Mask Area**'s color value will be used as **Basic Value**. Color values within the **Basic Value±Tolerance** range can be added to or wiped off from the segmentation data. The default **Mask Area** is 3\*3, other options are 1\*1, 5\*5, 7\*7;


**RGB**: The average **RGB** values of the **Mask Area**;

**Tolerance**: There are 3 **Tolerance** values, they are **R**, **G** and **B**. User can make fast and accurate object segmentation by selecting a proper **Tolerance** value according to their experience. The default **R**, **G** and **B** **Tolerance** values are 10;

 **Def...**: Used to mark the color of the segmentation area; The default **Color** is green;


 **Options...**: When clicking the **Options** button, a **Count Options** dialog as below will pop up. This dialog is the same as that in **Process>Segmentation & Count>Watershed (W)...**. Please refer to **Process>Segmentation & Count>Watershed (W)...** for the detailed operation of this dialog;

## Process

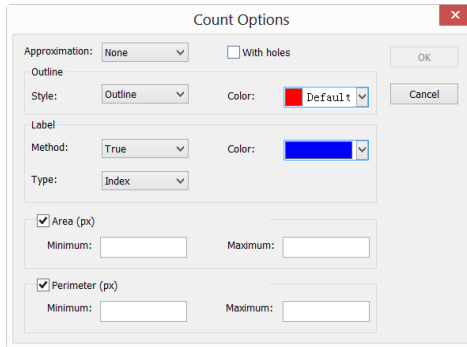


Here is an example to demonstrate the [Color Cubic](#) segmentation process:


1. [Open](#) an image as below:

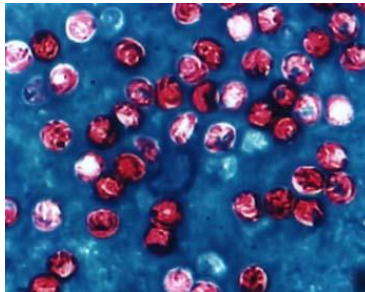

2. Because of the inevitable noise in the image, an image smooth operation should be done first. There are many algorithms to perform the image smooth operation and here we are to process it as follows: choose [Process>Filter](#) menu and click [Morphological](#) property page and a dialog will pop up with parameters as shown in the figure below on the left side. Click [OK](#) and the final smoothed image is shown below on the right side.

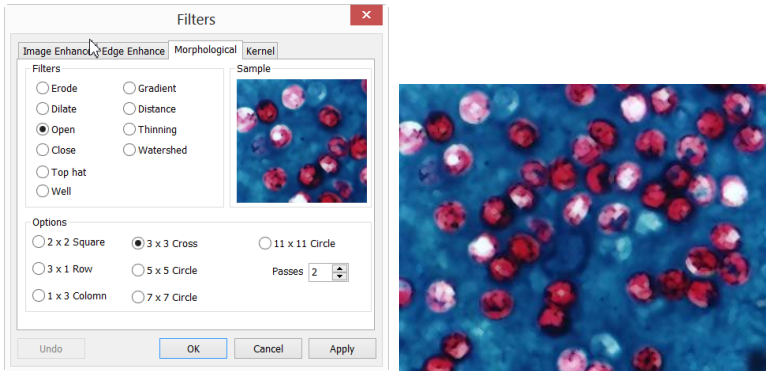


3. Choose **Process>Segmentation & Count> Color Cube...**, a **Color** dialog will pop up as shown below;

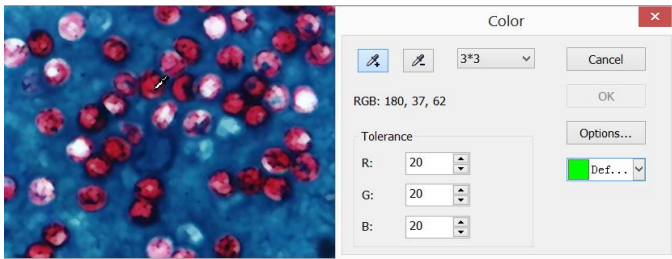


4. At this moment, the **Colorizing Pipette** is checked. Click the pixel wish to segment. That is to say, select the color area which is interested in. If some undesirable color area is included in the segmentation area, just check the **De-Colorizing Pipette** and click the undesirable pixels, thus the undesirable pixels will be wiped off. When the segmentation process is completed, click **OK** and the **Segmentation & Count** operation will be carried out.


## Process

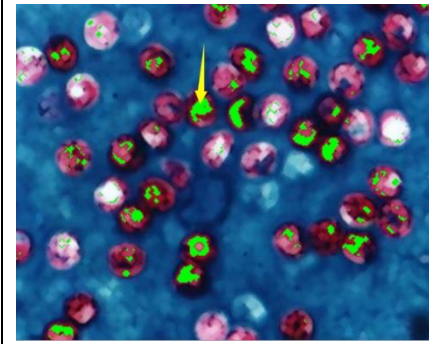


The result of segmentation after the first clicking at the pointed area with [Colorizing Pipette](#)

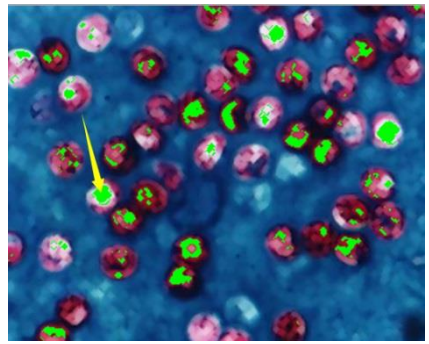

The result of segmentation after the second clicking at the pointed area with [Colorizing Pipette](#)

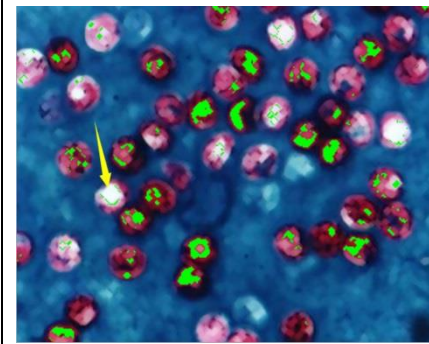


The result of segmentation after the second with the [De-Colorizing Pipette](#) (slight difference exists as inaccuracy in position)

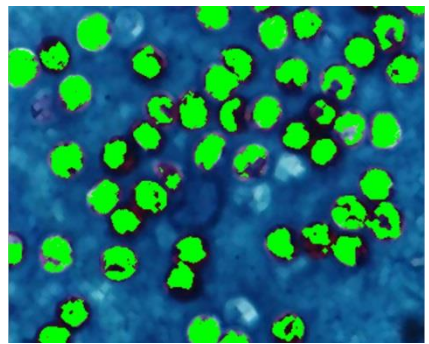

The result of segmentation after countless clicking with [Colorizing Pipette](#)

5. Click [Options](#) to set [Outline](#), [Label](#) and etc., the final results is shown below. So far the primary segmentation is completed.

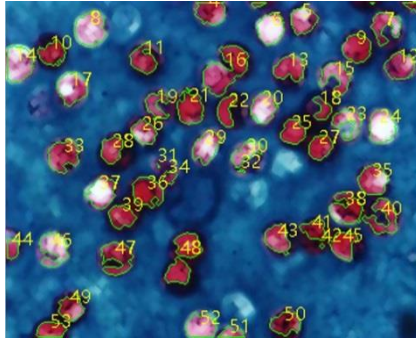


### 13.6.7 Split Objects(S)


It can be found out in this segmentation, particle #16 (located in the upper middle of the image) is not a single object but actually two separate one. However they have been calculated as a single object. Choosing [Split Objects](#) will correct this problem. Object splitting with [Split Objects](#) is discussed below.

As is shown in the image below, move the cursor onto target #16. Click the left mouse button and draw a straight line.


When pressing down the left mouse button, the cursor should not touch the target — the starting point of the split line should be off the target that is to be separated. Move the cursor to the bottom right of the target — the ending point of the split line should also be off the target that is to be separated. Release the left mouse button when this operation is completed. A split line is shown between the two adhesive objects as shown below:

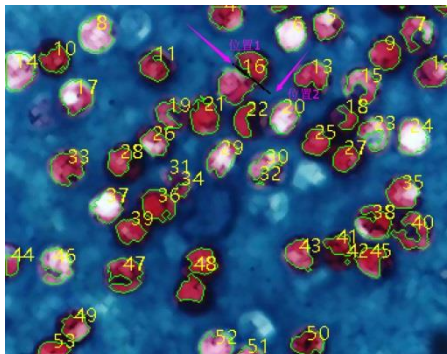

After the left mouse button is released, [ImageView](#) will re-count the whole image. The result of re-counting is shown as below. The previous #16 turns out to be #12 and #17 now:

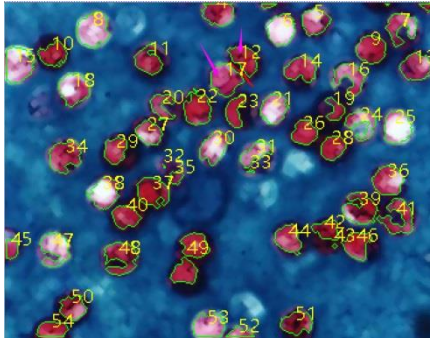

Unchecking or choosing [Split Objects](#) menu again will hide the split line. The final result of hiding the split line is shown as below. The whole [Split Objects](#) process is completed when the split line is hidden.

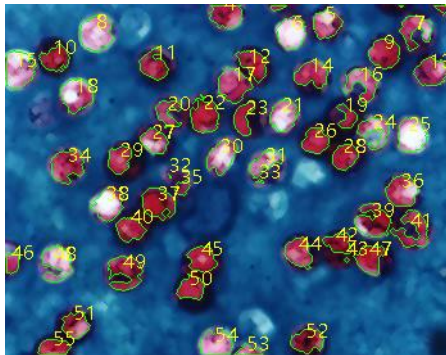

### 13.6.8 Count Result (T) ●●●

[Count Result](#) is a way to show count statistical result of the current image. [Count Result](#) dialog includes [Index](#)、[Center](#)、[Radius](#)(major-minor axis or non), [Area](#) and [Perimeter](#), as is shown below. The unit of statistical result is the same as what the user selects in the Unit for the displayed image. Click [Index](#)、[Center](#)、[Radius](#) (major-minor axis or none), [Area](#) and [Perimeter](#) and the statistical result will be automatically sorted according to their data. Choosing a certain item can check the

split object in the image. In the meanwhile, Index (or [Area](#) and [Perimeter](#)) of the other targets will be hidden automatically.

Index	Center	Radius	Area	Perimeter
1	(108.82, 96.30)	0.54	0.25	2.41
2	(51.32, 95.94)	0.98	0.75	4.11
3	(119.61, 95.57)	3.32	12.82	20.68
4	(60.67, 94.36)	6.18	59.16	41.91
5	(37.57, 90.30)	1.42	0.25	5.69
6	(29.81, 89.42)	0.57	0.31	2.62
7	(66.49, 85.19)	0.57	0.06	2.62
8	(25.06, 89.02)	5.78	76.52	45.86
9	(82.24, 93.40)	12.06	173.82	101.48
10	(15.70, 84.66)	4.50	1.62	20.56
11	(13.58, 82.36)	6.21	53.00	44.11
12	(12.70, 76.54)	0.73	0.62	3.41
13	(41.45, 80.95)	6.13	60.03	52.35
14	(2.65, 78.66)	5.95	64.70	40.29
15	(14.29, 72.84)	0.57	0.19	2.62
16	(83.97, 76.58)	6.20	66.13	55.76
17	(105.80, 81.50)	16.57	309.87	189.77
18	(17.99, 70.02)	7.26	82.86	62.48
19	(8.82, 65.61)	1.54	0.10	6.00

The [Center](#) column in [Result](#) is relevant to the [Approximation](#) option in the [Options](#) dialog. When selecting [Circle](#), radius of the circle will be listed as [Radius](#) column and when choosing [Ellipse](#), major-minor [Axis](#) of the [Ellipse](#) will be listed as [Axis](#) column; when selecting [None](#), no column shows up.

Click [Export](#) and then the statistical result, together with the image of [Segmentation & Count](#), will be exported to an [Excel](#) sheet for further analysis and processing.

### 13.7 Denoise(D)

[ImageView](#) provides 3 types of noise removal methods, [Adaptive Wiener Filter](#), [Bilateral Filter](#), [Non Local Means](#). The processing speed of the 3 methods is from fast to slow, and the denoising quality is getting better and better. Each method is described in detail in the following:

#### 13.7.1 Adaptive Wiener Filter(A)

The [Adaptive Wiener Filter](#) can preserve more image details than those of median filter, mean filter, Gauss filter. The effect is more remarkable for additive noise (such as Gaussian noise) and multiplicative noise (such as Poisson noise).

For the [Adaptive Wiener Filter](#) algorithm, please find the details in the relevant literatures, here only to illustrate the improvement of Adaptive Wiener Filter over the classical Wiener filter.


In the classical Wiener filter, the image noise intensity requires the user to manually input, but it is difficult to accurately enter the accurate value even for experienced users, because the value is usually very small, such as 0.0036781. Therefore in the development of the [Adaptive Wiener Filter](#), the noise level is automatically calculated according to the image mean variance.

The process is quite simple, open an image, choose the [Process>Denoise>Adaptive Wiener Filter](#) to denoise the image.

### 13.7.2 Bilateral Filter(B)●●●

The [Bilateral Filter](#) is a nonlinear filtering method that considers image spatial proximity, pixel value similarity, image spatial information and gray level similarity to achieve the purpose of edge preserving denoising. The [Bilateral Filter](#) has the simple, non-iterative, local characteristics. The [Bilateral Filter](#) is good to preserve image edge compare with Wiener filter or Gauss filter.

Choosing [Process>Denoise>Bilateral Filter●●●](#) will pop-up dialog called [Bilateral Filter](#) as shown below:

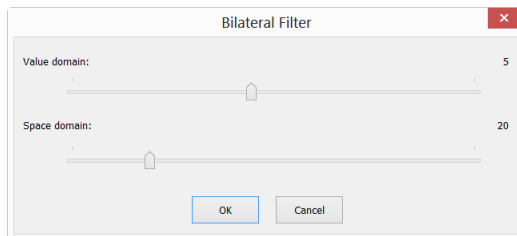

[Value domain](#): the range of neighborhood pixel in radius for considering, the greater the value, the slower process speed.

[Space domain](#): Sigma value, the higher the value, the more effective the denoising effect.


### 13.7.3 Non Local Means(NLM)●●●

The traditional local mean filter is a pixels average method around the target pixel, but the Non Local Means is a weighted average method to average all of the image patches over the search window. The weight is determined according to the similarity between the target patch and neighborhood patches in the search window.



Compared to other famous denoising algorithms, such as Gaussian, Wiener filter, total variation and wavelet denoising, The Non Local Means method can get better effect.

Choosing **Process>Denoise>Non Local Means** will pop-up dialog called **Non Local Means** as shown below:

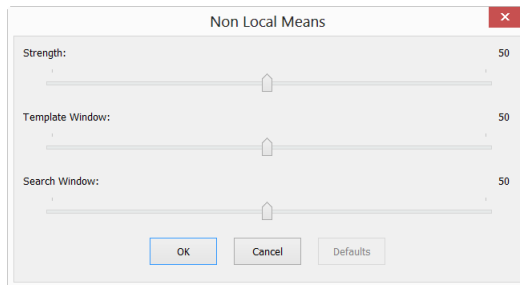

**Strength**: The denoising strength, the greater the value, the more removal the image noise, but will lose more details;

**Template Window**: The template block size, used to calculate the weight, the recommended default value is 7;


**Search Window**: The template patch search window size, used to calculate the weighted average value among image patches. Large value will increase the processing time. The recommended default value is 21.

### 13.8 Sharpen(N)

#### 13.8.1 USM(U)

**UnSharp Masking (USM)** is an image sharpening technique, often available in digital image processing software. The "unsharp" of the name derives from the fact that the technique uses a blurred, or "unsharp", positive image to create a mask of the original image. The unsharped mask is then combined with the negative image, creating an image that is less blurry than the original one.


Open an image and then choose **Process>Sharpen>USM** command, a dialog will pop up as below.

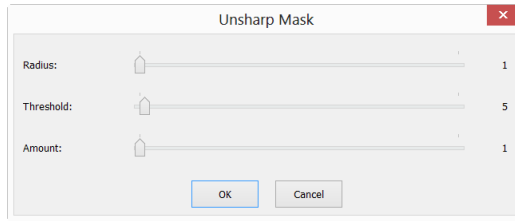

**Radius:** Affects the size of the edges to be enhanced, so a smaller radius enhances smaller-scale detail. Higher Radius values can cause halos at the edges. As a result, fine detail needs a smaller Radius. In addition, Radius and Amount interact; reducing one allows more of the other.

**Threshold:** Controls the minimum brightness change that will be sharpened. This parameter is important to prevent smooth areas from becoming speckled. The threshold setting can be used to sharpen more-pronounced edges, while leaving subtler edges untouched. Low values should sharpen more because fewer areas are excluded. Higher threshold values exclude areas of lower contrast.

**Amount:** is listed as a percentage, and controls the magnitude of each overshoot (how much darker and how much lighter the edge borders become). This can also be thought of as how much contrast is added at the edges. It does not affect the width of the edge rims.

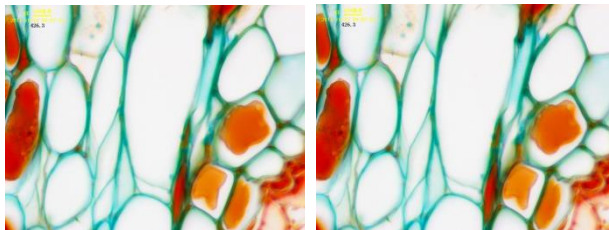


a) Original image; b) Sharpened image

### 13.8.2 Laplacian Sharpen(L)

The **Laplacian** operator is an example of a second derivative method of enhancement. It is particularly good at finding the fine detail in an image. Any feature with a sharp discontinuity (like noise, unfortunately) will be enhanced by a **Laplacian** operator. Thus, one application of a **Laplacian** operator is to restore fine detail to an image which has been smoothed to remove noise.

Open an image and then choose **Process>Sharpen>Laplacian Sharpen**, no parameter is required for this method.

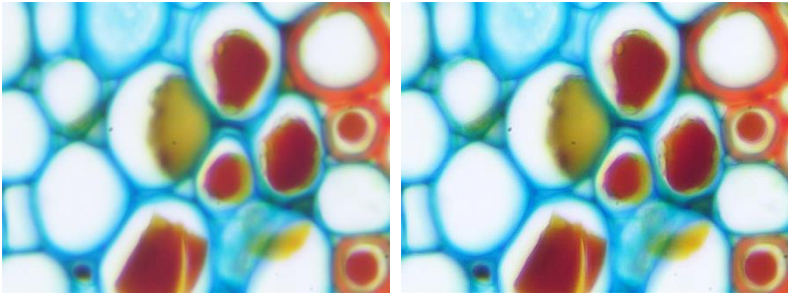


a) Original image; b) Sharpened image

### 13.9 Color Toning(G)

#### 13.9.1 Gamma(G)●●●



The **Process>Color Toning>Gamma●●●** measures the brightness of midtone values produced by a device (often a monitor). A higher gamma value yields an overall darker image.

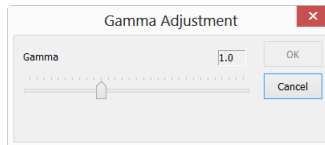

**Preview:** Check this button to display the real-time effects when one changes the slider bar's position. Default is checked;

**Gamma:** Dragging the slider bar to the left decreases the level, while moving it to the right increases the level. Values can range from 0 to 3.0. Default is 1.0.


#### 13.9.2 Histogram Equalization(Q)●●● **Shift+Q**

Adaptive histogram equalization (AHE) is a computer image processing technique used to improve contrast in images. It differs from ordinary histogram equalization (HE) in the respect that the adaptive method computes several histograms, each corresponding to a distinct section of the image, and uses them to redistribute the lightness values of the image. It is therefore suitable for improving the local contrast. However, AHE has a tendency to over amplify noise in relatively homogeneous

## Process

regions of an image. A variant of adaptive histogram equalization called contrast limited adaptive histogram equalization (**CLAHE**) prevents this by limiting the amplification.

Please open an image and then choose **Process>Color Toning >Histogram Equalization**, a dialog should pop up as follows.

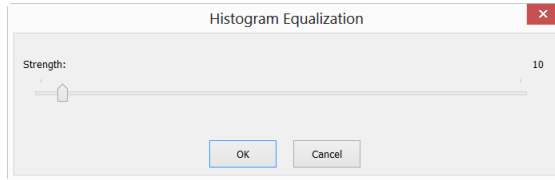

**Strength:** The **Strength** will affect the enhancement effect. The larger the value, the more obvious the effect.



a) Original image; b) Enhanced image

### 13.9.3 LCC

The **Local Color Correction** algorithm is computed in two steps:


A mask image is computed from the input image.

The mask image is computed from the intensity component of the color image, defined as the average of R, G and B values i.e.  $I=(R+G+B)/3$ . The use of intensity information avoids distortions of the chroma. The mask image is obtained by inverting and then blurring the intensity component of the input image.

The input and mask images are combined to get the result.

The combination operation consists of a power function, where the exponent is computed using the mask value previously found. If the mask value is greater than 128, it will result in an exponent less than 1, while if the mask value is lower than 128, it will result in an exponent greater than 1. Moreover, if the mask value is precisely 128, the exponent will be 1, and it will have no effect on the input image. The operation is equivalent to a pixel-wise gamma correction.

Please open an image and then choose **Process>Color Toning >LCC•••**, a dialog should pop up as follows.

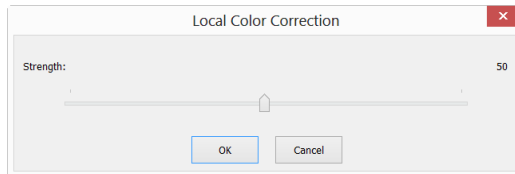

**Strength:** The strength will affect the enhancement effect. The larger the value, the more obvious the effect. Range:1~100, default is 50.



a) Original image; b) Enhanced image

### 13.9.4 AMSR

There are limited dynamic range problems when real world scenes are captured from a digital camera and displayed on monitors. Tone mapping algorithms are applied to image processing to reduce the dynamic range of an image to be displayed on low dynamic range devices. Multi-scale Retinex is one of the most popular methods for dynamic range compression, color constancy and color rendition. Here, we improve its performance by adopting the adaptive weight functions, named Adaptive Multi-scale Retinex (AMSR).

Please open an image and then choose [Process>Color Toning>AMSR](#), the a) Original image; b) Enhanced image




a) Original image; b) Enhanced image

### **13.10 Filter(I)●●●      Shift+I**

Choose the [Process>Filter●●●](#) command to apply one of [ImageView](#)'s numerous filters on the active image. If you are not familiar with the process and effects of filtering, some discussions about spatial filtering should be reviewed. [ImageView](#) provides an extensive set of convolution and non-convolution (morphological) filters. You can also create custom filter kernels and apply them with the [Filter](#) commands.

Choosing the [Process>Filter●●●](#) command will open the [Filter](#) dialog. Each group of filters has its own property page or tab, where the [Filter](#) type and size can be selected. The filtered results are almost always written to the active image. The [Edit>Undo](#) command can be used to remove [Filter](#) operations that have been applied.

#### **13.10.1 Image Enhance**

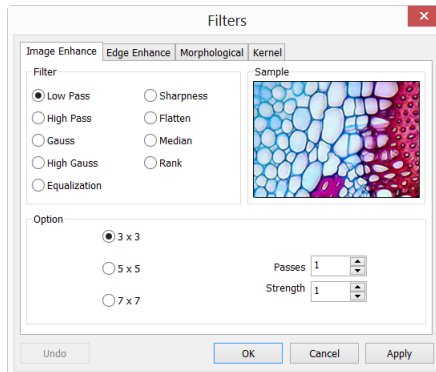

**Low Pass:** Check this filter to soften an image by eliminating high-frequency information (this has the effect of blurring sharp edges). The **Low Pass** filter replaces the center pixel with the mean value in its neighborhood. The **Low Pass** filter can also be used to remove noise.

**High Pass:** Check this filter to enhance high-frequency information. The **High Pass** filter replaces the center pixel with a convolved value that significantly increases its contrast from its neighbors. The **High Pass** filter leaves only elements of high contrast.

**Gauss:** Check this filter to soften an image by eliminating high-frequency information using a **Gauss** function. This has the effect of blurring sharp edges. The operation of the **Gauss** filter is similar to the **Low Pass** filter, but it degrades the image less than the **Low Pass** filter.

**High Gauss:** Check this filter to enhance fine details. This operation is similar to the unsharp masking technique (see the Sharpen filter), but it introduces less noise into the image. It uses a Gaussian curve type of kernel. Available in 7x7 and 9x9 kernel sizes.

**Equaliza-tion:** This filter is used to enhance the contrast based on the histogram of the local neighborhood (See **Option** below).

**Sharpness:** Check this filter to enhance fine details, or refocus an image that is blurred. The sharpen filter sharpens the image using the unsharp masking technique.

**Median:** Check this filter to remove impulse noise from an image. The **Median** filter replaces the center pixel with the **Median** value in its neighborhood. It will also blur the image.

**Rank:** Check this filter to remove impulse noise from an image. The pixels in the kernel are ranked by order of intensity, and the pixel in that range at the rank percentage is chosen for comparison. For example, in a 5x5 kernel, there are 25 pixels. A rank percentage of 95% would choose second-brightest pixel for comparison. If the difference between the selected pixel and the center pixel is greater than the threshold value, the **Rank** filter replaces the value of the center pixel with the value of the selected pixel.

**Option :1.** If one of the **Enhancement** filters is checked, the following options will be displayed:

**3 x 3:** Check **3 x 3** kernel will produce a more subtle filtering effect.

**5 x 5:** Check **5 x 5** kernel will produce a moderate filtering effect.

**7 x 7:** Check **7 x 7** kernel will produces a more extreme filtering effect.

**Passes:** Set the filter applied times on the image. When a filter is applied multiple times, its effect is amplified by each pass. An image that has been softened by one pass of the **Low Pass** filter will be softened further by a second pass.

**Strength:** Enter an applied value from 1-10 that reflects how much of the filtering effect on the image.

A value of 10 specifies the full strength (100%) of the filtered result applied to each pixel. Values less than 10 cut the full weight of the filter.

A value of 1 indicates that only 10% of the difference between the filtered pixel value and the original pixel value should be applied, a value of 2 indicates that 20% of the difference should be applied, and so forth.

**Rank:** This value specifies which pixel in the sorted array will be used to replace the center pixel. Pixels in the array will be sorted in ascending order. The pixels are indexed from 0 to **Kernel Size** x **Kernel Size**-1. In the pixel index 0 corresponds to the lowest pixel value.



The **Rank** will be specified in terms of a percentage of the indexes (**Kernel Size** x **Kernel Size-1**). A 50% **Rank** means the middle of the array. 0% rank means the lowest index (lowest gray value), and 100% rank means the highest index (highest gray value).

**Option: 2.** If the **Equalization** filter is checked, the options will relate to the histogram equalization. **Local Histogram Equalization** modifies the contrast of an image based on the pixel values in a small window surrounding each pixel.

**Window:** Image pixels statistics (min, max, histogram, mean, standard deviation, etc.) will be calculated on a small **Window** of the image. These measurements are then used to derive the local contrast for that area of the image. In short, an area of **Window x Window** around each pixel is all that is considered when modifying the intensities in the image. Larger **Window** produces smoother results, while small **Window** track small details more closely.


**Best Fit:** Choose the **Best Fit** button to optimize the values for the particular image. The results are achieved by stretching the local histogram to maximize the contrast between the brightest and darkest pixels in the local window region.

**Linear:** This option distributes the histogram linearly across the intensity scale. This function produces a high contrast image with the highest possible dynamic range.

**Logarithmic:** This option concentrates the histogram at the low end of the scale. This function produces a high contrast image with little dynamic image. It will tend to darken the image overall. It is useful for increasing the contrast in a very light image.

**Exponential:** This option concentrates the histogram at the high end of the scale. This function produces a high contrast image with little dynamic image. It will tend to lighten the image overall. It is useful for increasing the contrast in a very dark image.

### **13.10.2 Edge Enhance**

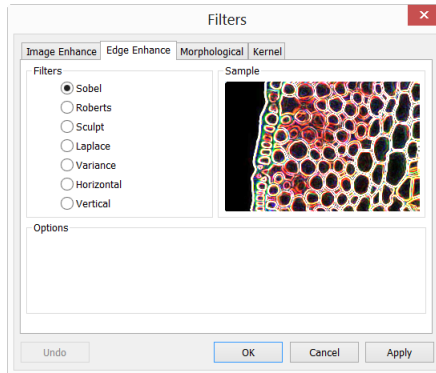

**Sobel** : Check this filter to enhance just the principal edges in an image. The **Sobel** applies a mathematical formula to a 3x3 neighborhood to locate and highlight its edges.

**Roberts**: Check this filter to enhance fine edges in an image. The **Roberts** filter is not a convolution filter. It applies a mathematical formula upon a 4 x 4 neighborhood to produce its effect. The upper left pixel in the neighborhood is the one that is replaced.

**Sculpt**: Check this filter to apply a sculpted effect on the image.

**Horizontal**: Check this filter to detect and emphasize horizontal edges.

**Vertical**: Check this filter to detect and emphasize vertical edges.

**Options** : 1. If one of the **Edge** filters has been checked, the options will relate to kernel size and filtering strength. The following options will be displayed:

**3 x 3**: Check 3x3 kernels to produce a more subtle filtering effect.

**5 x 5**: Check 5x5 kernels to produce a moderate filtering effect.

**7 x 7**: Check 7x7 kernels to produce a more extreme filtering effect.


**Passes**: Enter the number of times that the filter will be applied to the image. When a filter is applied multiple times, its effect is amplified by each pass. An image that has been softened by one pass of the **Image Enhancement Filter**, will be softened further by a second pass.

**Strength**: Enter a value from 1-10 that reflects how much of the filtering effect to

apply to the image. A value of 10 specifies that the full strength (100%) of the filtered result will be applied to each pixel. Values less than 10 cut the full weight of the filter - a value of 1 indicates that only 10% of the difference between the filtered pixel value and the original pixel value should be applied, a value of 2 indicates that 20% of the difference should be applied, and so forth.

Option 2. If **Sobel** or **Roberts** is checked, no options are available.

### 13.10.3 Morphological

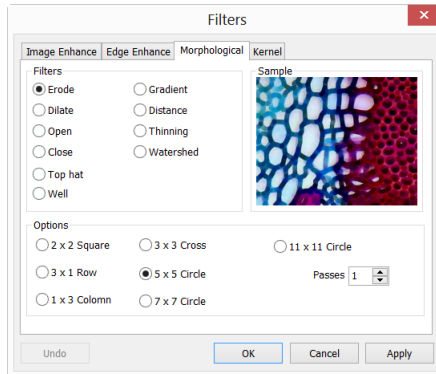

**Erode:** Check this morphological filter if one wants to modify the size of objects in the image. The Erode filter erodes the edges of bright objects and enlarges the edges of dark ones.

**Dilate:** Check this morphological filter if one wants to modify the size of objects in the image. The Dilation filter dilates bright objects and erodes dark ones.

**Open:** Check this morphological filter if one wants to modify the shape of objects in the image. Assuming the image contains bright objects on a dark field, the Open filter will smooth object contours, separate narrowly connected objects, and remove small dark holes.

**Close:** Check this morphological filter if one wants to modify the shape of the objects in the image. Assuming the image contains bright objects on a dark field; the **Close** filter will fill gaps and enlarge protrusions to connect objects that are close together.

**Tophat:** Check this filter to detect and emphasize points, or grains, that are brighter than the background. There are 3 kernel sizes for this processing. Click the radio

button to change the kernel size to the value that most closely matches the size of the grains to detect.

**Well:** Check this filter to detect and emphasize points, or grains, that are darker than the background. There are 3 kernel sizes for this processing. Click the radio button to change the kernel size to the value that most closely matches the size of the grains to detect.

**Gradient:** Check this filter to enhance edges in an image.

**Watershed:** Check this filter to separate objects that are touching. The Watershed filter erodes objects until they disappear, then dilates them again, but will not allow them to touch. The Watershed filter will not operate upon True Color images. If one wants to separate objects in a True Color image, he must first convert it to **Gray Scale** (see **Process Frame: Image>Gray Scale**).

**Thinning:** Check this filter to reduce an image to its skeleton. When choosing this filter, one must set the threshold that determines whether a pixel is part of the subject or part of the background (see Options below). The Thinning filter will not operate upon True Color images. If one wants to thin a **True Color** image, he must first convert it to **Gray Scale**.

**Distance:** The distance filter is used to show the distances of pixels within blobs to the outer boundaries of those blobs. After applying the distance filter, the background will be black (i.e. pixels with value 0). Only the area within the blobs will have non-zero values (will be white). The values of each pixel within the blob will be a count of the shortest distance from that pixel to the edge of the blob. Thus, all pixels along the blob's border will have a value of 1 (since they are one pixel away from the edge of the blob); pixels that are a distance of 2 from the border will have the value 2, and so on. This creates a distance map of the image. The **Distance** filter will not operate upon **True Color** images. If one wants to use the **Distance** filter with a **True Color** image, he must first convert it to **Gray Scale**.

**Options 1.** If **Erode**, **Dilate**, **Open**, or **Close** filters is checked, the options will relate to the kernel size and shape. The following options will be presented:

**2 x 2 Square:** Check to use the 2x2 square kernel configurations.

**3 x 1 Row** : Check to use the 3x1 row kernel configuration.

**1 x 3 Column** : Check to use the 1x3 column kernel configuration.

**3 x 3 Cross** : Check to use the 3x3 cross kernel configuration.

**5 x 5 Circle** : Check to use the 5x5 circular kernel configurations.

**7 x 7 Circle** : Check to use the 7x7 circular kernel configurations. This is a two-pass filter, accomplished using a 5 x 5 circle followed by a 3x3 cross.

**11 x 11 Circle** : Check to use the 11 x 11 circular kernel configurations. This is a three-pass filter, accomplished using a 5 x 5 circle followed by another 5 x 5 circle, followed by a 3 x 3 cross.

**Passes**: Set the number of times iterate the filter.

**Note**: The circular kernels are especially effective on round objects (cells, grains and so on) because their circular configuration preserves the circular shape of the objects better than square configurations.

**Option 2**. If the [Tophat](#), [Well](#), or [Gradient](#) filter is selected, the options will relate to kernel size and shape. The following options will be presented:

**3 x 3**: Check to use the 3x3 square kernel configurations.

**5 x 5**: Check to use the 5x5 square kernel configurations.


**7 x 7**: Check to use the 7x7 square kernel configurations.

**Option 3**. If [Watershed](#), [Thinning](#), or [Distance](#) filter is checked, the options will relate to the threshold. The following option will be presented:

**Threshold**: Enter a percentage value from 1-100 that specifies the intensity value to binarize the image. For example, a Threshold of 50% on a [Gray Scale](#) image would set all values  $\leq 127$  to 0 (black) and all values  $\geq 128$  to the maximum value for that image class (white).

### 13.10.4 Kernel

The [Kernel](#) page allows edit the kernel files for the morphological and convolution filters.

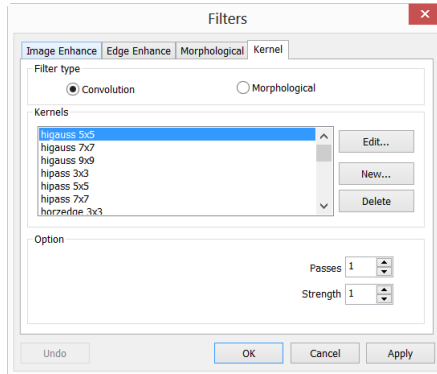

**Note:** The **HiPass**, **LowPass**, **Laplacian** and **Unsharp** kernel files are used by the **HiPass**, **LowPass**, **Laplacian**, and **Sharpen** options listed in the **Image Enhancement Filters** page dialog window (i.e. there is no difference between selecting one of these kernel files and selecting its **Option** button in the **Filter** window -- the 2 methods ultimately do the same thing). Because these kernel files are essential to the operation of these filtering options, they must not be deleted or renamed.

**Filter type:** Check to modify the kernel for a selected **Filter type**, either **Convolution** or **Morphological** filters.

**Edit•••:** Invoke the **Edit** Kernel dialog to modify the selected filter kernel.

**Name•••:** This combobox contains the name of the selected kernel file. If one wants to save the modified kernel file to the same file, leave it as is. If one wants to save the file to a new location, enter the new filename here.

**Kernel Size:** Click the spin buttons or enter the number to change the size of the kernel. Either direction may take into account one to nine pixels. As one modifies the **Kernel Size**, the shape of the kernel representation changes accordingly. In the center of the dialog, there are white boxes containing coefficients that will be multiplied with each pixel that will be taken into account by the filter kernel. One can change any coefficient by clicking on it and adjust it as desired.

**Fill:** Click this button to fill every element of the kernel with a particular value. The Fill kernel dialog appears. One may enter a value between 0 and 10. Using the Fill button is useful for setting all coefficients to the same value. One may

then change the coefficients that require a different value.

**Offset:** The pixel whose value is being modified is usually the center-most pixel. One may, however, designate any pixel. ImageView signals the pixel to be changed by putting a box around it. Choose the **X** and **Y Offset** spin buttons to apply

**New•••:** Click to create a new filter kernel. The **Edit Kernel** dialog will appear. The functions of the dialog are the same way as the dialog for **Edit•••** described above), with the exception that the file name for the new kernel file must be provided.

**Delete:** Click to delete the selected filter kernel file.

**Options:** The choices in this group box will vary depending upon the kind of selected filter.

### 13.11 Image Stacking(S)•••




The image-stacking method is a form of speckle imaging commonly used for obtaining high quality images from a number of short exposures with varying image shifts. It has been used in astronomy for several decades, and is the basis for the image stabilization feature on some cameras. The method involves calculation of the differential shifts of the images. This is easily accomplished in astronomical images since they can be aligned with the stars. Once the images have aligned, they are averaged together. It is a basic principle of statistics that variation in a sample can be reduced by averaging together the individual values. In fact, when using an average, the signal-to-noise ratio should be increased by a factor of the square root of the number of images.


Image stacking can also be used for biological microscope image and florescent microscope image to increase the image SNR and dynamical ranges; this is why we introduce image stacking into **ImageView**.

**ImageView Image Stacking** introduced advanced image matching techniques for rotated, shifted and scaled images. The user can record a short video to get a high quality stacked image at ease without considering the image rotation, shifting and scaling between a series of images in the video. The steps of Image Stacking are described as below:


1. Choose **Processing>Image Stacking** menu, a Windows **Open** dialog will pop up as shown below;

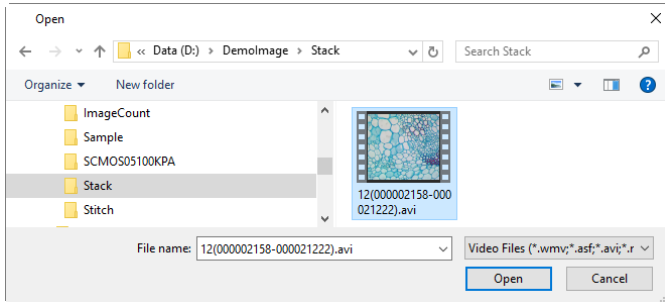

2. Choose the right video file recorded before in the **Open** dialog, here we can open "test.avi" for demonstration, click **Open** to open the avi file;
3. Then an **Image Stacking** dialog will pop up to show the progress of the each image's stacking progress.

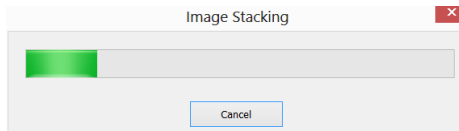

4. If **Cancel** is pressed, the **Image Stacking** will be canceled. After the stacking is finished, a stacked image will be displayed in a new window for further application. The final image is shown as below. One can find the stacked image signal to noise ratio is greatly improved. From the stacked image has some black edges, this is because the images in the video is moved and in the stacking process, ImageView will added 0 to the image area that has no corresponding pixel in the reference image (we choose the first image in the video file as the reference image).






**Note:** a. [ImageView](#) support wmv, asf, avi, mp4, m4v, 3gp, 3g2, 3gp2, 3gpp, mov, mkv, flv, rm, rmvb for [Image Stacking](#) operation; b) In the [Image Stacking](#) process, [ImageView](#) takes the first frame as the reference image, this means the first frame is very important and should be assure the first frame to be the right image scene and the subsequent frames have a greater overlap region with the first frame.

### 13.12 Line Profile(L)●●●


Choose the [Process>Line Profile●●●](#) command to illustrate how pixels along a selected line are distributed by graphing the number of pixels at each color intensity level.

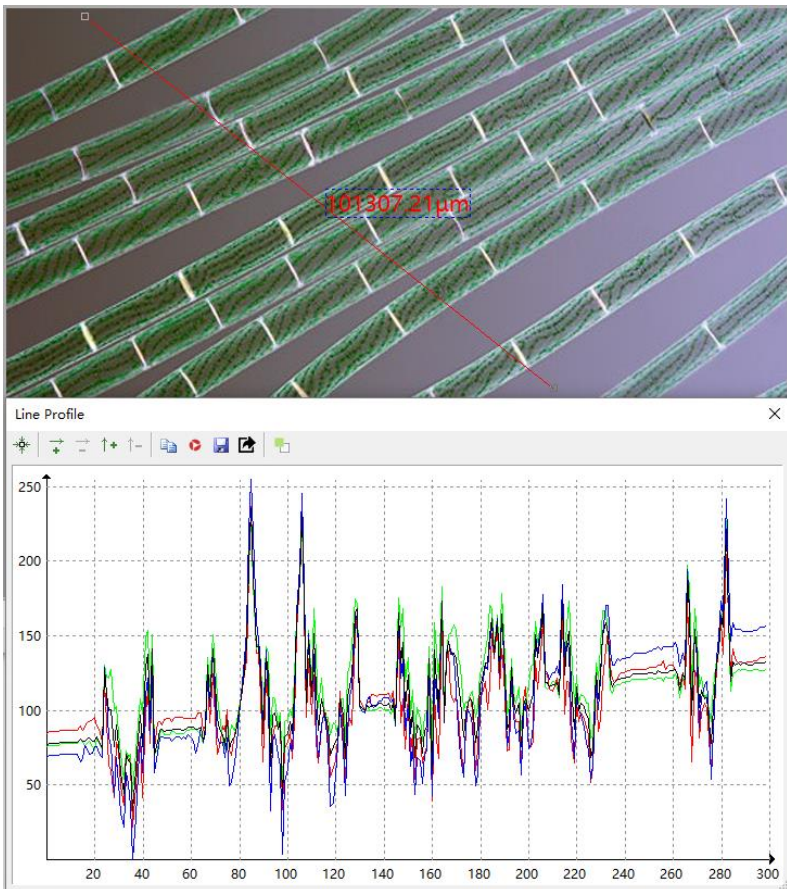

Choose the [Measurements>Arbitrary Line](#), or [Measurements>Horizontal Line](#) or

[Measurements> Vertical Line](#) command to draw a line on the image and choosing the [Process>Line Profile](#) will bring up a [Line Profile](#) dialog as above(The procedure can be inversed):

In a [Line Profile](#) dialog, the horizontal axis represents the spatial scale, and the vertical axis represents the intensity values which range from 0 to 255. If the image is a gray scale image, the gray value will be profiled. If the image is a HSV color image, the R,G,B and the brightness values will be profiled separately with the

corresponding R, G,B and black colors. Its toolbar 

button functions are as follows:



: Fit the current [Line Profile](#) window to the best scale;



: Zoom in the current horizontal axis;



: Zoom out the current horizontal axis;



: Zoom in the current vertical axis;



: Zoom out the current vertical axis;



: Copy the [Line Profile](#) window's content onto the clipboard;



: Capture the image in the [Line Profile](#) window as a new untitled image;




: Save the [Line Profile](#) image in bmp format;



: Export the current Y axis values of R,G,B and brightness to the \*.txt file.




: Open the windows color dialog to set the background color of the profile window;

Only when the line is selected, the Line Profile can be painted in the window. Using [Object Select](#) button  on the toolbar to select the line over the image or video window.

### 13.13 Surface Plot●●●

The [Process>Surface Plot●●●](#) (or 3-D Plot) tool creates a 3-D representation of the intensity of an image. When choosing the [Surface Plot](#) command, keep in mind that X=image width and Y=image height, and Z=pixel gray value.

In the viewpoint window, the [elevation](#) and [rotation](#) of the image can be adjusted by dragging the mouse on the image.

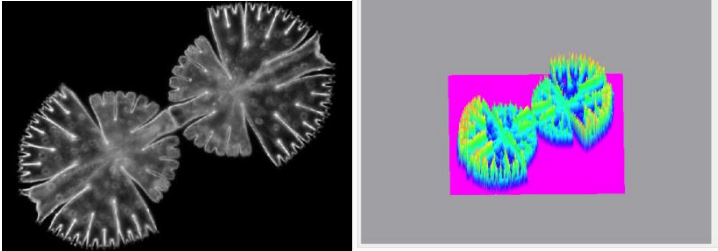

**Position Solid:** The left edit control indicates the relative position of the entire image in the viewpoint window, whose default value is 0.5. The right edit control indicates the relative height of the display of the Z scale, whose default value is 1.

**Reset:** Set the **Position Solid**'s two edit controls to their default values.

**Image Background Color:** Choose this command to display a color dialog where one can adjust the background color of the viewpoint window.


**Capture:** **Capture** the active image in the viewpoint window as a new image.

**Color Table:** Select the colors to map the gray values found in the surface plot. The button at each end of the **Color Table** brings up the color dialog, which allows select the start and end colors of the range. (Please refer to **Pseudo Color** for more information)

### 13.14 Pseudo Color(P)●●●



**Note:** Image must be in **Gray Scale**.

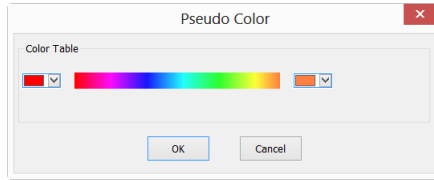Choose the **Pseudo Color** command to "colorize" the active monochromatic image. This is used to highlight certain features in a gray scale image such as display all densities above a certain point in red, or, the imaging device recorded thermal information, all temperatures below a certain point can be revealed in blue color.



When **Pseudo Color** a monochromatic image, a special palette need to be build with which the monochromatic image is displayed. **Pseudo Coloring** an image does not modify the pixels' values in image bitmap (it does not convert image to true color or palette). It simply associates a **Pseudo Color** palette with the image that interprets the gray-level values in the image as color.


Pseudo Colored images are very similar in structure to palette class images, but they differ in a couple of important ways. First, the pixels' values in a **Pseudo Colored** image actually represent continuous-tone intensity information, whereas a palette image's pixels carry no intensity significance. Secondly, a palette image includes a palette table that is actually part of the image file.

The colors used to map the gray values can be selected. The buttons at each end of the color strips (  or  ) will bring up the color dialog separately, which allows select the start and end colors of the range.



### 13.15 Range●●● Shift+R

The **Process>Range●●●** command allows set the intensity levels of the image to increase the contrast and enhance the display in low-light situations. Choose the **Range** command to open the **Range** dialog.

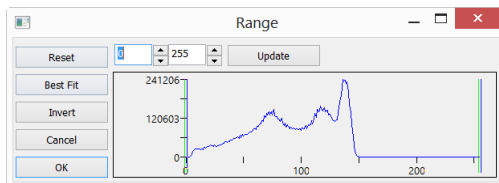

Two **vertical markers** show the **upper** and **lower** limits of the intensity levels. These markers can be moved with mouse through the drag and drop method. For a color image, the histogram will reflect the **red**, **green**, and **blue** values with corresponding

colors lines.

Two **Edit** controls indicate the values of the intensity levels. Choose the spin buttons to increase or decrease these values. All values between 0 and the lower limit will be black and all values between the upper limit and the upper end of the scale will be white. These two edit control values corresponding to the two **vertical markers** show the **upper** and **lower** limits of the intensity levels. Defaults are 0 and 255 respectively.

**Reset:** The **Reset** button allows **Reset** the black and white levels to the high and low ends of the dynamic **Range**.


**Best Fit:** The **Best Fit** button automatically sets the intensity levels to the **Best Fit**. **Best Fit** instructs **ImageView** to optimize the brightness and contrast values for the particular image.

**Invert:** The **Invert** button reverses the color of the image.

**Update:** **Update** will refresh the display **Range** with the most current image information.

### 13.16 Binary(B)●●● Shift+B

**Binary** is a kind of gray level process. If the gray of the pixel is greater than the given threshold, the pixel's color will be changed into white. Otherwise, the pixel's color will be changed into black. Although the process may lose some information, it is an important step of other processes.

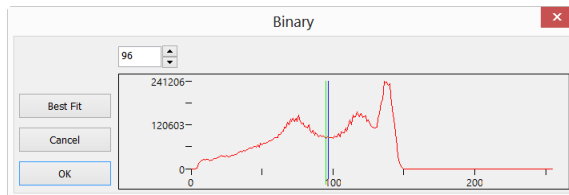

The curve on the **Binary** dialog shows the gray distribution of the image.

The **Line** in the dialog indicates the threshold value. Drag the line to change the threshold, or change the value in the **Line** position **edit** box (in the top left corner of the dialog) to move the **Line**.

The **Line** position **edit** box shows the current position value of the **Line**; Modify the


value will move the [Line](#) at the same time;

Click the "[Best Fit](#)" button to apply the auto threshold process to the image. It uses an automatic threshold to make the image [Binary](#).

## 14 Layer

### 14.1 About layer

[ImageView](#)'s [Layer](#) is like sheets of stacked acetate. You can see through transparent areas of a [Layer](#) to the [Layers](#) below. You add a [Layer](#) to position the [Objects](#) content on the [Layer](#), like sliding a sheet of acetate in a stack. You can also hide/show a layer to make content invisible/visible.

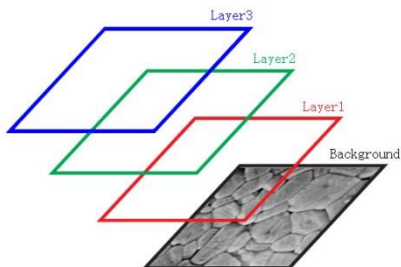

You use layers to perform tasks such as perform the [Measurement](#) on the image without polluting the image and save it for the future adjustment or further analysis.

### 14.2 Organizing layers

A new image has a single [Layer](#) called [Background](#) layer. The number of additional layers you can add to an image is limited only by your computer's memory.


You work with layers in the [Layers Sidebar](#). The [Layer Sidebar](#) help you organize and manage layers just like the [Layer](#) menu.

### 14.3 Layers for non-destructive measurement and label

Rather than edit image pixels directly, you can label the image with text and measure the image and leave the underlying pixels unchanged. Because of the non-destructively to images, you can later tweak or remove the label and the [Objects](#).

### 14.4 Layer Sidebar

# Layer

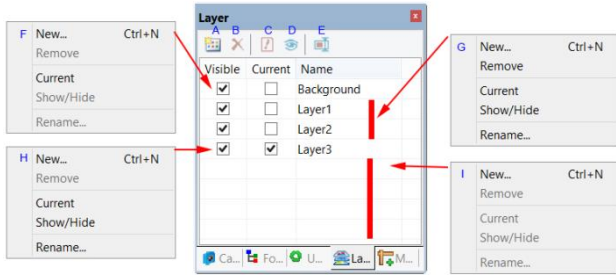

- A: Make a **New** layer;
- B: **Remove** a layer;
- C: Set the **Current** layer;
- D: **Show/Hide** a layer;
- E: **Rename** a layer;
- F: Right mouse button context menu for the **Background** layer;
- G: Right mouse button context menu for the **Current** not checked layer;
- H: Right mouse button context menu for the **Current** checked layer;
- I : Right mouse button context menu in the blank area;

**Note:** a). Only one layer can be checked as **Current Layer**. If a layer's "**Current**" is checked, the **Visible** will be checked automatically; b). The **Current** and **Background** layers cannot be removed. Only the non-current and non- background layers can be removed; c). All the **Objects** on the **Current Layer** can be selected, edited or exported; d). The non-current **Layer** can be **Visible** (checked) or invisible (unchecked).

## 14.5 Layer menu and layer sidebar page context menu

The function of the **Layer** menu and **Layer Sidebar** right mouse button context menu are the same. They are:



### 14.6 New(N)●●●



**Ctrl+N**

Setup a new layer. After the new layer is setup, it will be added to the end of the **Layer Sidebar**'s items and the **Visible** and **Current** will be checked.

### 14.7 Remove(R)●●●





Remove the non-current Layer.

**Note:** the Background and Current Layer cannot be removed.

### 14.8 Current(C)●●●



Set the selected layer as the Current Layer. User then can edit the Object on the Current Layer or added new Object on the Current Layer.

### 14.9 Show/Hide(S)●●●



Set the non-current Layer visible or invisible. The Current Layer cannot be toggled between Visible and invisible state. It is always Visible.

### 14.10 Rename(E)●●●



Rename a Layer.

### 14.11 Export to Image(M) F2


Export all the layers' Objects to the image, this will pollute the image and cannot be recovered anymore.

### 14.12 Export to Microsoft Excel●●●



F3

Export the image plus all the Objects on the Current Layer to the Excel file.

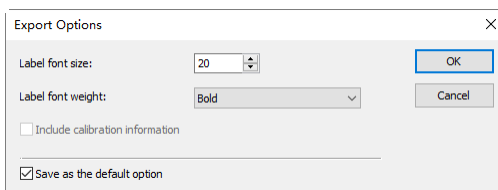

**Label font size:** Used for the Measurement Object's label font size, the default value is 20(8~72);

**Label font weight:** Normal, Bold, Heavy. The default is Bold;

**Include calibration information:** If the images are calibrated, check this item will output the calibration information in the Excel file;

**Save as the default option:** If this item is checked, the current setting will be saved for the future application;

### 14.13 Export all to Microsoft Excel●●●




F4

## Layer

---

Export the current opened different images which have **Objects** on their **Layer** to a single **Excel** file. This function can be used to capture images with measurement objects from different video field of view who may have the same characteristic. The output in the **Excel** file then can be processed to get the statistic properties.

The menu will be active only when 2 or more images are opened and have **Measurement Objects** over the images.

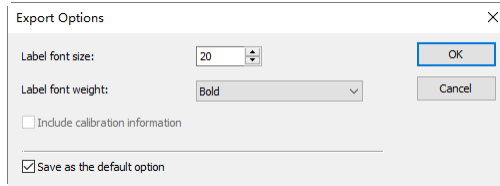

**Label font size:** Used for the **Measurement Object's** label font size, the default value is 20(8~72);


**Label font weight:** Normal, Bold, Heavy. The default is Bold;

**Include calibration information:** If the images are calibrated, check this item will output the calibration information in the Excel file;

**Save as the default option:** If this item is checked, the current setting will be saved for the future application;

## 15 Measurements

The [Measurements](#) menu is mainly used for the image measurement. With this menu, you can measure the image with many geometrical shape at ease. [ImageView](#) use [Layer](#) technique to manage the measurement object. This will never pollute the image pixels. The [Measurements](#) menus and its submenus are shown below.

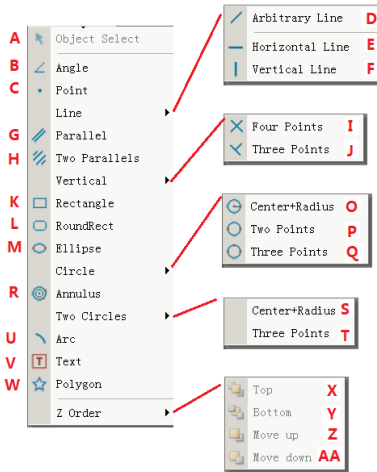


About the [Layer](#) technique, please check the [Layer](#) menu and [Layer Sidebar](#) in Sec.14.

About the [Measurements](#) setup, please check [Options>Measurement...](#) and [Measurement Sidebar](#) in [View>Sidebar](#) menu in Sec.8.

About the [Measurements](#) menu's toolbar buttons, please check [ImageView](#)'s toolbar in Sec.4: UI toolbar.

### 15.1 Object Select(S)

The [Measurements>Object Select](#) menu or the toolbar button  will be enabled only when a new [Measurement](#) is made over the [Background Layer](#).

After the [Measurement](#) is done on the specific layer, choose this menu to select the [Objects](#).

1. The [Object](#) can be selected by clicking on it;

2. Select a group of **Objects** by including them in a rectangular area with **Object Select** command or by press down the **Shift** key and clicking the **Object** with left mouse button until all the desired **Objects** are selected.

**Note:** a) To check or modify the parameters of the selected **Object**, just select a single **Object** and the **Measurement Sidebar** will be activated automatically. Here you can edit the corresponding object parameters to modify its properties; b) The **Appearance**, **Coordinates** on **Measurement Sidebar** will be enabled only when a single **Object** is selected. The **Calculation** will be effective for a single selected **Object** or multiple selected **Objects**. Its calculated items will depend on the selected **Object** type (The type could be the same or different).

### 15.2 Angle(N)



#### 15.2.1 Angle (3 Points)



1. Move the mouse on the image to point 1, mark it by clicking the left mouse button;
2. Move the mouse to point 2, mark it by clicking the left mouse button;
3. Move the mouse to point 3, mark the final point by clicking the left mouse button. A label  $50.26^\circ$  will be shown near point 2;

#### 15.2.2 Angle (4 Points)



1. Move the mouse on the image to point 1, mark it by clicking the left mouse button;
2. Move the mouse to point 2, mark it by clicking the left mouse button; Point 1 and point 2 will be connected automatically to form L12

## Measurements


---

3. Move the mouse to point 3, mark the final point by clicking the left mouse button.

4. Move the mouse to point 4, mark it by clicking the left mouse button; Point 3 and point 4 will be connected automatically to form L34

After the above process, L12 and L34 will be extended with the dot line to form an angle between L12 and L34.

A label  $34.40^\circ$  will be shown near vertex;

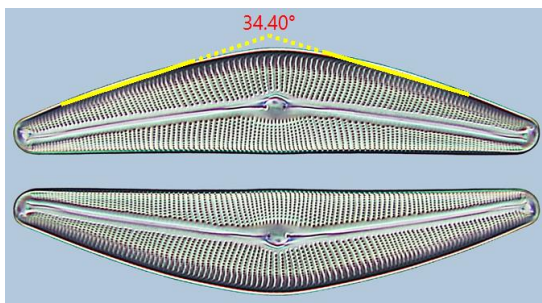

### 15.3 Point(P)



Move mouse to the point; click the left mouse to mark it. It will show the point **Label P<sub>n</sub>** and its position x and y over the image.

**Note:** a) To check or modify the parameters of the selected **Object**, just select a single **Object** and the **Measurement Sidebar** will be activated automatically. Here you can edit the corresponding **Object** parameters to modify its properties; b) The **Appearance**, **Coordinates** on **Measurement Sidebar** will be enabled only when a single **Object** is selected. The **Calculation** will be effective for a single selected **Object**

or multiple selected **Objects**. Its calculated items will depend on the selected **Object** type (The type could be the same or different).


### 15.4 Line(L)

#### 15.4.1 Line>Arbitrary Line(A)



Draw **Arbitrary Line** between the two points on the specified layer.

1. Choose the **Measurements>Line> Arbitrary Line** command;
2. Move mouse to the 1st point; click the left mouse to mark it;
3. Move mouse to the 2nd point, click the left mouse to mark it again, a line with L1 and its length will be shown.

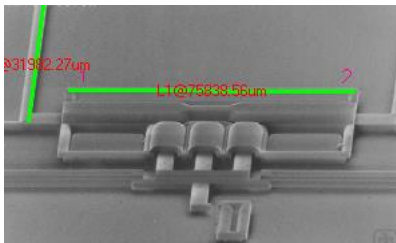

**Note:** a) To check or modify the parameters of the selected **Object**, just select a single **Object** and the **Measurement Sidebar** will be activated automatically. Here you can edit the corresponding **Object** parameters to modify its properties; b) The **Appearance**, **Coordinates** on **Measurement Sidebar** will be enabled only when a single **Object** is selected. The **Calculation** will be effective for a single selected **Object** or multiple selected **Objects**. Its calculated items will depend on the selected **Object** type (The type could be the same or different).

#### 15.4.2 Line> Horizontal Line(H)



Draw a **Horizontal Line** between the two points on the specified layer. When the 1st point is marked, the 2nd point's y coordinate will be restricted to equal to the first point's y coordinate automatically.

**Note:** a) To check or modify the parameters of the selected **Object**, just select a single **Object** and the **Measurement Sidebar** will be activated automatically. Here you

can edit the corresponding **Object** parameters to modify its properties; b) The **Appearance**, **Coordinates** on **Measurement Sidebar** will be enabled only when a single **Object** is selected. The **Calculation** will be effective for a single selected **Object** or multiple selected **Objects**. Its calculated items will depend on the selected **Object** type (The type could be the same or different).

### 15.4.3 Line> Vertical Line(V)




Draw a **Vertical Line** between the two points on the specified layer. When the first point is marked, the second point's x coordinate will be restricted to equal to the first point's x coordinate automatically.

**Note:** a) To check or modify the parameters of the selected **Object**, just select a single **Object** and the **Measurement Sidebar** will be activated automatically. Here you can edit the corresponding **Object** parameters to modify its properties; b) The **Appearance**, **Coordinates** on **Measurement Sidebar** will be enabled only when a single **Object** is selected. The **Calculation** will be effective for a single selected **Object** or multiple selected **Objects**. Its calculated items will depend on the selected **Object** type (The type could be the same or different).

### 15.5 Parallel(R)



1. Choose the **Measurements>Parallel** command;
2. Move mouse and click to mark the 1st point;
3. Move mouse and click to mark the 2nd point;
4. Move mouse and click to mark the 3rd point;
5. Move mouse again, one will find the 4th point is always restricted to parallel to the line connecting point 1 and point 2. Click to mark the 4th point. Two parallel lines will be labeled and numbered.

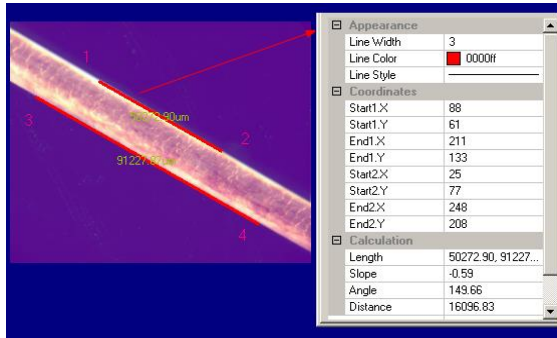

**Note:** a) To check or modify the parameters of the selected **Object**, just select a single **Object** and the **Measurement Sidebar** will be activated automatically. Here you can edit the corresponding **Object** parameters to modify its properties; b) The **Appearance**, **Coordinates** on **Measurement Sidebar** will be enabled only when a single **Object** is selected. The **Calculation** will be effective for a single selected **Object** or multiple selected **Objects**. Its calculated items will depend on the selected **Object** type (The type could be the same or different).


### 15.6 Two Parallels(O)



1. Move mouse and click its left button to mark the 1st point.
2. Move mouse and click its left button to mark the 2nd point. Line 1 (the 1st line) connect these two points will be overlaid on the image
3. Move mouse and click its left button to mark the 3rd point.
4. Move mouse again, one will find the 4th point is always restricted to parallel to the Line 1 connecting point 1 and point 2. Click to mark the 4th point. Line 2 will be drawn which is parallel to Line 1. A dot line DL 1 located at the center of Line 1 and Line 2 will also be marked. Thus the 1<sup>st</sup> parallel is finished.
5. Repeated step 1~4 will draw Line 3 and Line 4. A dot line DL 2 located between the center of Line 3 and Line 4 will also be marked. Thus the 2nd parallel is finished.
6. **ImageView** will label the distance between DL1 and DL2 in with Unit specified in the Unit combo box. The final result is shown below:



## Measurements

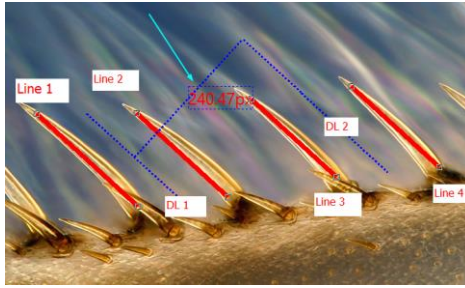

### 15.7 Vertical(V)



#### 15.7.1 Vertical>Four Points.



1. Move mouse and click its left button to mark the 1st point.
2. Move mouse and click its left button to mark the 2nd point. A line (the 1<sup>st</sup> line) connect these two point be overlaid on the image
3. Move mouse and click its left button to mark the 3rd point.
4. Move mouse again, one will find the 4th point is always restricted to perpendicular to the line of point 1 and point 2. Click to mark the 4th point. Two vertical lines will be labeled and numbered.

**Note:** a) To check or modify the parameters of the selected **Object**, just select a single **Object** and the **Measurement Sidebar** will be activated automatically. Here you can edit the corresponding **Object** parameters to modify its properties; b) The **Appearance**, **Coordinates** on **Measurement Sidebar** will be enabled only when a single **Object** is selected. The **Calculation** will be effective for a single selected **Object** or multiple selected **Objects**. Its calculated items will depend on the selected **Object** type (The type could be the same or different).


### 15.7.2 Vertical>Three Points



1. Move mouse and click its left button to mark the 1<sup>st</sup> point;
2. Move mouse and click its left button to mark the 2<sup>nd</sup> point. A line (the 1<sup>st</sup> line) connecting these two points will be overlaid on the image;
3. Move mouse and click its left button to mark the 3<sup>rd</sup> point. The 2<sup>nd</sup> line will be overlaid on the image which is perpendicular to the 1<sup>st</sup> one.

**Note:** a) To check or modify the parameters of the selected **Object**, just select a single **Object** and the **Measurement Sidebar** will be activated automatically. Here you can edit the corresponding **Object** parameters to modify its properties; b) The **Appearance**, **Coordinates** on **Measurement Sidebar** will be enabled only when a single **Object** is selected. The **Calculation** will be effective for a single selected **Object** or multiple selected **Objects**. Its calculated items will depend on the selected **Object** type (The type could be the same or different).

### 15.8 Rectangle(T)

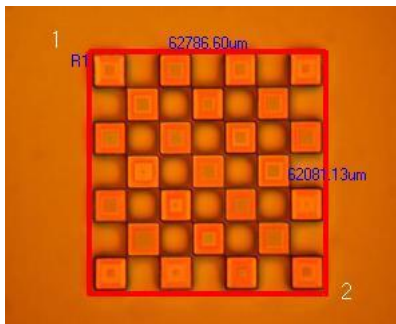

1. Move mouse to the 1st point; click its left mouse button to mark it;
2. Move mouse to the 2<sup>ed</sup> point; click its left mouse button to mark it. A **Rectangle** will be overlaid on the image according these two diagonal points.


**Note:** a) To check or modify the parameters of the selected **Object**, just select a single **Object** and the **Measurement Sidebar** will be activated automatically. Here you can edit the corresponding **Object** parameters to modify its properties; b) The

Appearance, Coordinates on Measurement Sidebar will be enabled only when a single Object is selected. The Calculation will be effective for a single selected Object or multiple selected Objects. Its calculated items will depend on the selected Object type (The type could be the same or different).

### 15.9 Ellipse(I)



1. Choose the **Measurements>Ellipse** command;
2. Move mouse to mark the 1st point;
3. Move mouse to mark the 2nd point;
4. If it is not superposing with the shape on the image, choose the **Measurements>Object Select** command to adjust the position to adjust the Ellipse in order to coincide with the image shape.

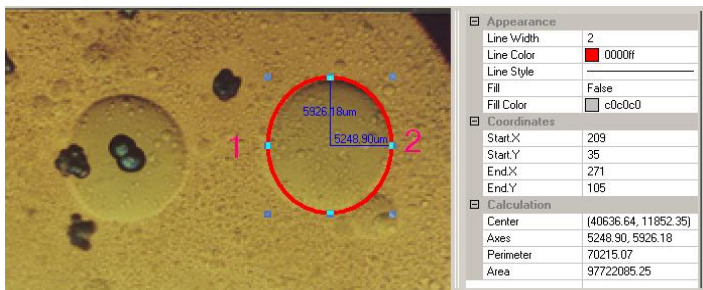

**Note:** a) To check or modify the parameters of the selected Object, just select a single Object and the Measurement Sidebar will be activated automatically. Here you can edit the corresponding Object parameters to modify its properties; b) The Appearance, Coordinates on Measurement Sidebar will be enabled only when a single Object is selected. The Calculation will be effective for a single selected Object or multiple selected Objects. Its calculated items will depend on the selected Object type (The type could be the same or different).

### 15.10 Circle(C)




#### 15.10.1 Circle>Center+Radius



## Measurements

---

Choose the **Measurements>Circle>Center+Radius** command to draw a circle with **Center+Radius** method on the specified **Layer**. Its radius is [C1@33583.88um](#).



**Note:** a) To check or modify the parameters of the selected **Object**, just select a single **Object** and the **Measurement Sidebar** will be activated automatically. Here you can edit the corresponding **Object** parameters to modify its properties; b) The **Appearance**, **Coordinates** on **Measurement Sidebar** will be enabled only when a single **Object** is selected. The **Calculation** will be effective for a single selected **Object** or multiple selected **Objects**. Its calculated items will depend on the selected **Object** type (The type could be the same or different).

### 15.10.2 Circle>Two Points



Choose the **Measurements>Circle>Two Points** command to draw a circle with **Two Points** method on the specified layer.

**Note:** a) To check or modify the parameters of the selected **Object**, just select a single **Object** and the **Measurement Sidebar** will be activated automatically. Here you can edit the corresponding **Object** parameters to modify its properties; b) The **Appearance**, **Coordinates** on **Measurement Sidebar** will be enabled only when a single **Object** is selected. The **Calculation** will be effective for a single selected **Object** or multiple selected **Objects**. Its calculated items will depend on the selected **Object** type (The type could be the same or different).

### 15.10.3 Circle>Three Points



Choose the **Measurements>Circle>Three Points** command to draw a circle with **Three Points** method on the specified layer.


**Note:** a) To check or modify the parameters of the selected **Object**, just select a single **Object** and the **Measurement Sidebar** will be activated automatically. Here you can edit the corresponding **Object** parameters to modify its properties; b) The

**Appearance**, **Coordinates** on **Measurement Sidebar** will be enabled only when a single **Object** is selected. The **Calculation** will be effective for a single selected **Object** or multiple selected **Objects**. Its calculated items will depend on the selected **Object** type (The type could be the same or different).

### 15.11 Annulus(U)



1. Find the **Annulus** center 1 and click mouse button to mark the **Annulus** center;
2. Move mouse to let the first circle superpose with the image circle, clicking the mouse left button;
3. Move mouse to let the second circle superpose the image circle, clicking the left mouse button. Two radiuses with number and the units will be displayed on the **Annulus**;



**Note:** a) To check or modify the parameters of the selected **Object**, just select a single **Object** and the **Measurement Sidebar** will be activated automatically. Here you can edit the corresponding **Object** parameters to modify its properties; b) The **Appearance**, **Coordinates** on **Measurement Sidebar** will be enabled only when a single **Object** is selected. The **Calculation** will be effective for a single selected **Object** or multiple selected **Objects**. Its calculated items will depend on the selected **Object** type (The type could be the same or different).

### 15.12 Two Circles(W)



#### 15.12.1 Two Circle>Center+Radius(R)

Draw two circles with **Center+Radius** method on the specified layer. After the two circles are drawn, a line connecting these two circle centers will be drawn.

**Note:** a) To check or modify the parameters of the selected **Object**, just select a single **Object** and the **Measurement Sidebar** will be activated automatically. Here you


can edit the corresponding **Object** parameters to modify its properties; b) The **Appearance**, **Coordinates** on **Measurement Sidebar** will be enabled only when a single **Object** is selected. The **Calculation** will be effective for a single selected **Object** or multiple selected **Objects**. Its calculated items will depend on the selected **Object** type (The type could be the same or different).

### 15.12.2 Two Circle>Three Points(3)

Draw two circles with **Three Points** method on the specified layer. After the two circles are drawn, a line connecting these two circle centers will be drawn.

**Note:** a) To check or modify the parameters of the selected **Object**, just select a single **Object** and the **Measurement Sidebar** will be activated automatically. Here you can edit the corresponding **Object** parameters to modify its properties; b) The **Appearance**, **Coordinates** on **Measurement Sidebar** will be enabled only when a single **Object** is selected. The **Calculation** will be effective for a single selected **Object** or multiple selected **Objects**. Its calculated items will depend on the selected **Object** type (The type could be the same or different).

### 15.13 Arc(A)



1. Move mouse to mark the 1st point;
2. Move mouse to mark the 2nd point;
3. Move mouse to mark the 3rd point, then an **Arc** with **Label** and its **Length** will be drawn connecting these three points.


**Note:** a) To check or modify the parameters of the selected **Object**, just select a single **Object** and the **Measurement Sidebar** will be activated automatically. Here you can edit the corresponding **Object** parameters to modify its properties; b) The **Appearance**, **Coordinates** on **Measurement Sidebar** will be enabled only when a

single **Object** is selected. The **Calculation** will be effective for a single selected **Object** or multiple selected **Objects**. Its calculated items will depend on the selected **Object** type (The type could be the same or different).

### 15.14 Text(X)



1. Choose the **Measurements>Text** command;
2. Move mouse to mark the 1st point;
3. Move mouse to mark the 2nd point, a rectangle with dash line restrict the **Text** window size. After the mouse button is released, a dialog called **Text** will bring up for you to enter the **Text** and define the **Text**, **Frame** styles and adjust the **Text** positions.
4. Enter the text and click the right mouse button to end the **Text** object.

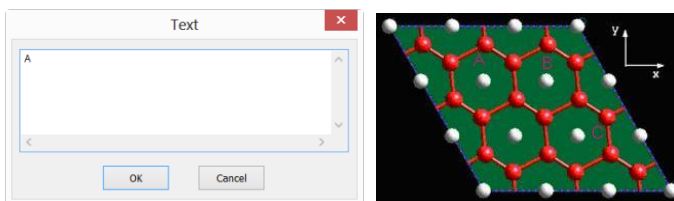


**Note:** a) To check or modify the parameters of the selected **Object**, just select a single **Object** and the **Measurement Sidebar** will be activated automatically. Here you can edit the corresponding **Object** parameters to modify its properties; b) The **Appearance**, **Coordinates** on **Measurement Sidebar** will be enabled only when a single **Object** is selected. The **Calculation** will be effective for a single selected **Object** or multiple selected **Objects**. Its calculated items will depend on the selected **Object** type (The type could be the same or different).

### 15.15 Polygon(G)



1. Choose the **Measurements>Polygon** command;
2. Move mouse and click the left mouse button to mark the 1st point;
3. Move mouse and click the left mouse button to mark the 2nd point.  
•••;

- n. Move mouse and click the left mouse button to mark the nth point;  
Click the right mouse button to end the **Polygon** command.




**Note:** a) To check or modify the parameters of the selected **Object**, just select a single **Object** and the **Measurement Sidebar** will be activated automatically. Here you can edit the corresponding **Object** parameters to modify its properties; b) The **Appearance**, **Coordinates** on **Measurement Sidebar** will be enabled only when a single **Object** is selected. The **Calculation** will be effective for a single selected **Object** or multiple selected **Objects**. Its calculated items will depend on the selected **Object** type (The type could be the same or different).

### 15.16 Curve(E)

#### 15.16.1 Curve>Model 1



1. Press down the left mouse button and move mouse according to the requirement to draw any curve in **Model 1** format.
2. If the mouse left mouse button is released and move the mouse to a new position and then click the left mouse button again will draw a line to connect the last point.
3. Release the left mouse button and click the right mouse button to end **Mode 1 Curve**.






### 15.16.2 Curve>Model 2



The **Model 2 Curve** operation is almost the same that of the **Polygon**,

1. Choose the **Measurements>Curve>Mode 2** command;
2. Move mouse to a point and click the left mouse button to mark the 1st point;
3. Move mouse to a point and click the left mouse button to mark the 2nd point.
4. ...;
- n-1. Move mouse to a point and click the left mouse button to mark the (n-1)th point;
- n. Move mouse to the final point and click the left mouse button to mark the nth point, then click the right mouse button to end the current **Mode 2 Curve** process.

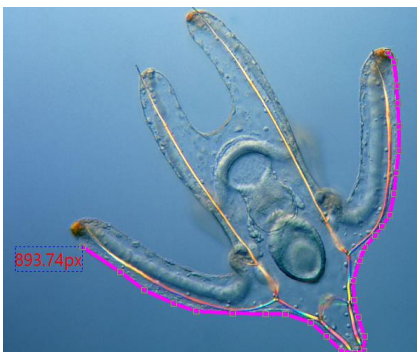


Choosing  button can adjust the finished **Model 2 Curve**.

### 15.17 Scale bar(B)




Choose the **Measurements>Scale bar** command will bring up a **Scale Bar** dialog as below:

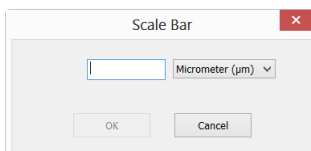


Input the number in the length edit box to determine the scale bar length. The **Unit** is chosen according to the current **Unit** in the **Options>Measurement>Length Unit**

## Measurements

page. If the **Unit** is pixel, then **Scale Bar** dialog will be change to

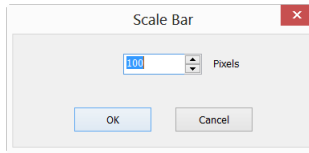

Change the default value(100) to the desired length or directly click **OK**, a **Scale bar** will display on the image in measurement style. One can move the **Scale bar** to where ever he wants(Choosing **Measurements>Object Select** after the **Scale bar** is displayed on the **Image** or **Video** window and move the mouse to the **Scale Bar** and click down the left mouse button). The final result should be:

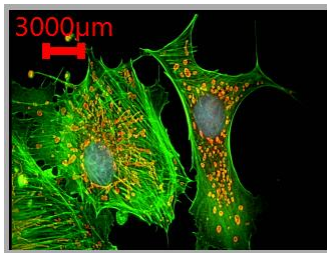


### 15.18 Arrow



Draw an Arrow on the image to specify the key point on the image or video.

### 15.19 Z Order(Z)

The Z Order submenu is shown below:



**Top:** Modify the selected **Object**'s relative position to the uppermost place of all **Objects** on the **Current** layer;

**Bottom:** Modify the selected **Object**'s relative position to the lowest place of all **Objects** on the **Current** layer;

**Move Up:** Modify the selected **Object**'s relative position to the higher place of the two on the **Current** layer;

## Measurements

---

**Move Down:** Modify the selected **Object**'s relative position to the lower place of the two on the **Current** layer;


## 16 Options

### 16.1 Preferences(P)●●●





There are 7 pages for the [Preference](#) dialog. They are [Quick Save](#), [File](#), [Print](#), [Grids](#), [Cursor](#), [Capture](#) and [Misc](#) pages.

#### 16.1.1 Quick Save Page

The [File>Quick Save](#) menu or the [Quick Save](#) icon  on the toolbar will be enabled when a) a new image window with the captured image from the camera; b) an image window is created by choosing the [File>Paste as New File](#) menu.

[File>Quick Save](#) can save the file at quick way with no need to specify the file directory, file name and file format. All those are specified in [Options>Preferences●●●>Quick Save](#) property page.

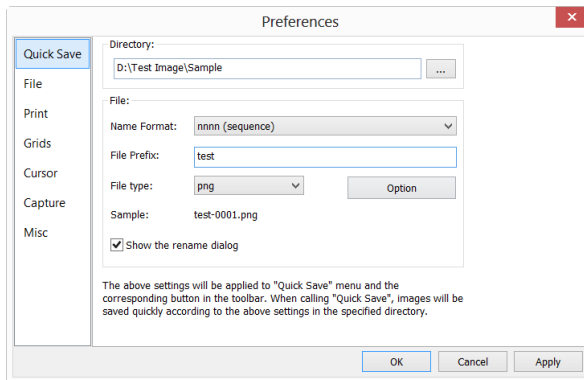

**Directory:** Enter the name of the drive and directory where the new image will be saved. You may either type the path information, or use the [Browse](#) button  to locate it from a standard [Browse Folder](#) dialog;

**Name Format:** The [year](#), [month](#), [date](#), [hour](#), [minute](#) and [second](#) or [nnnn\(sequence\)](#) are used as part of the file name. If more files are saved with in a second, a [\(xx\)](#) suffix is attached to the end of [Name Format](#) to avoid the possible name confliction. For the [nnnn\(sequence\)](#) [Name Format](#), no suffix is needed.


**File Prefix:** Enter a file name prefix for [Quick Save](#) when generating files names for a


series of images. This prefix will be combined with [Name Format](#) to form a final file name naming paradigm.

**File Type:** In this combobox, select the format in which you want the image to be saved (can be [BMP](#), [JPG](#), [PNG](#), [TIF](#)). Click [Option](#) button to set the different parameters for encoding the file (For [BMP format](#), the [Option](#) will be disabled. See [File>Save As...](#) menu about the details of the format encoding methods); If there are [Objects](#) over the image, the [File Type](#) will be chosen as "ImageView File Type (\*.tft)" by [ImageView](#).

**Sample:** The final file name is shown at the right of the [Sample](#) label for reference.

**Show the rename file dialog:** The file name can be renamed according to this item's setup. When this item is checked, a [Rename](#) dialog will pop up after choosing

[File>Quick Save](#) command or click the [Quick Save](#) icon  on the toolbar. The new name can be specified again according to the requirement.

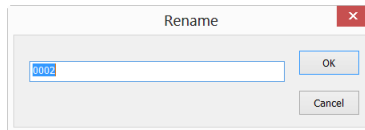

### 16.1.2 File Page

One can check a file [Extension](#) for the specified file [Format](#) and its [Abbr.](#)(abbreviation), to determine whether or not it will be displayed in the [Browse](#) window or not (The checked [Format](#) can be displayed in the [Browse](#) window).

**Extension:** Used to identify the file extension;

**Format:** English full name of file formats;


**Abbr.:** File [Format](#)'s abbreviation;

**Browse:** Check/uncheck to determine whether or not the file format can be displayed in the [Browse](#) window;

**Config...:** To configure the image file [Save As Option](#) for JPEG, Portable Network Graphics, Tag Image File Format, CompuServ, JPEG 2000 Standard, JPEG


## Options

Codestream. For details, please refer to the [Option](#) button explanation in the [File>Save As](#) dialog.

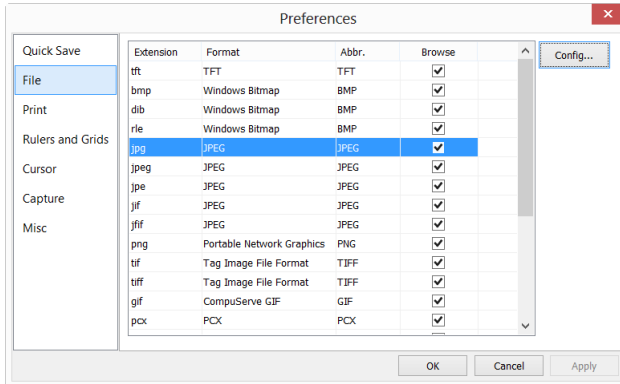

### 16.1.3 Print Page

One can set the [Page Header](#) and [Page Footer](#) in following format:

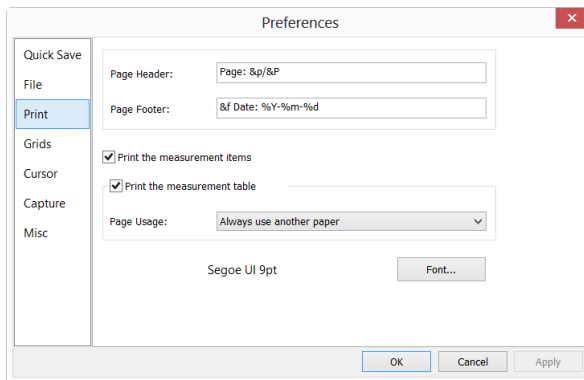

[&f](#) File Name

[&p](#) Current Page

[&P](#) Total Pages

[%A](#) Full weekday name

[%b](#) Abbreviated month name

[%B](#) Full month name

[%c](#) Date and time representation appropriate for locale

[%d](#) Day of month as decimal number (01 - 31)

[%H](#) Hour in 24-hour format (00 - 23)

## Options

---

[%I](#) Hour in 12-hour format (01 - 12)  
[%j](#) Day of year as decimal number (001 - 366)  
[%m](#) Month as decimal number (01 - 12)  
[%M](#) Minute as decimal number (00 - 59)  
[%p](#) Current local times A.M./P.M. indicator for 12-hour clock  
[%S](#) Second as decimal number (00 - 59)  
[%U](#) Week of year as decimal number, with Sunday as first day of week(00-53)  
[%w](#) Weekday as decimal number (0 - 6; Sunday is 0)  
[%W](#) Week of year as decimal number, with Monday as first day of week(00-53)  
[%x](#) Date representation for current locale  
[%X](#) Time representation for current locale  
[%y](#) Year without century, as decimal number (00 - 99)  
[%Y](#) Year with century, as decimal number  
[%z %Z](#) Time-zone name or abbreviation; no characters if time zone is unknown  
[%%](#) Percent sign

For example:

Choosing [&f Date:%Y-%m-%d](#) will print the file name and Date with yyyy-mm-dd format on the page header.

Choosing [Page:&p/&P](#) will print Page: 01/11 on the page footer(Suppose the current page is page 1 and the total pages is 11).

[Print the measurement item](#): If there are measurement item overlaid on the image, check it will print these objects on the image. [Measurement Sheet](#) on the page;

[Print the measurement table](#): If there are measurement item overlaid on the image, check it will print these objects' [Measurement Sheet](#) on the page with;

[Always use another paper](#): Print the [Measurement Sheet](#) data on a separate page;

[Auto](#): Print the [Measurement Sheet](#) data just behind the image (if the image and data can be arrange in a single page) of on a separate page (if not);


[Do not use another paper](#): Print the [Measurement Sheet](#) data just behind the image page;

**Font:** Choose the **Font** for the data.

### 16.1.4 Grids Page

Choosing the **View>Grid>Setting** command, or choosing the **Preference** command and clicking the **Grids** page realize the same function.

Choosing the **Preference** command and clicking the **Grids** page can set the **Grid Style**, **Line Style**, and **Line Color** for the **Grid** overlaid on the video and image window can also be set.

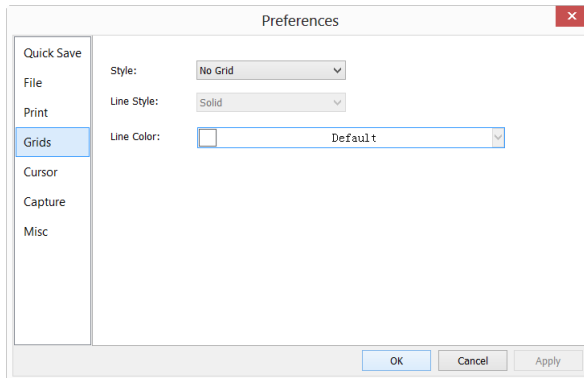

**Grid Style:** The **Grid Style** can be **No Grid**, **Auto Grid** or **Manual Grid**. Default is **No Grid**;

**Grid Line Style:** The **Line Style** for the grid can be **Solid**, **Dash**, **Dot** or **DashDot** et al. Default is **Solid**;

**Grid Line Color:** The color of the grid line. Default is Red (255,0,0).

### 16.1.5 Cursor Page

This command will set the mouse cursor for the video and image window operations.

Select the **Horizontal** cross in:

**None** (window default), **Single** (single line), **Double(1 Pixel)**, **Double(3 Pixels)**, **Double(5 Pixels)**, **Double(7 Pixels)**, and **Double(9 Pixels)** formats.

Select the **Vertical** cursor in:

**None** (window default), **Single** (single line), **Double(1 Pixel)**, **Double(3 Pixels)**,





Double(5 Pixels), Double(7 Pixels), and Double(9 Pixels) formats.

Single means single line. Double means two parallel lines. 1 Pixel means the line space between the two lines is 1 pixel in distance. The other sizes also have this meaning.


Select the cursor shape from Cross, Point, and Null.

In the figure below, a cursor with Double horizontal and vertical lines with 9 Pixels cross (for the alignment application, the longer one) and the Cursor as a Cross was defined

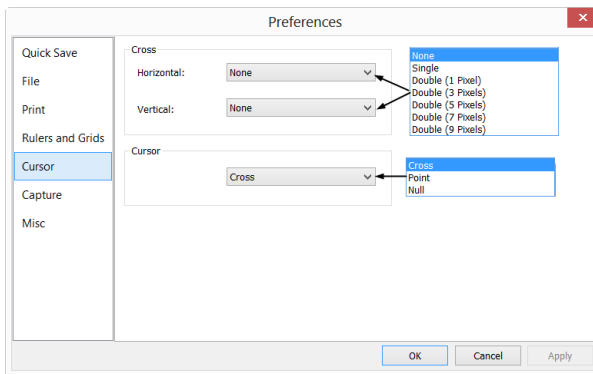


### 16.1.6 Capture Page

If one wish to capture an image with many Objects overlaid on the video window, the following settings should be defined first.


- 1.Choosing the Options>Preferences••>Capture command, a dialog called Preferences will be brought up as shown below;
- 2.Clicking the Capture page and then checking Capture with Marker and Watermark or Capture with Measurement;
- 3.Click Ok to end the setup, or Apply to apply the setup, or Cancel to cancel the setup.
- 4.After the above steps are finished, if there are Marker, Watermark or Objects overlaid above the video, choosing the Capture>Capture Image or clicking  Snap on the Camera Sidebar will capture the image with Marker, Watermark or Objects

overlaid on the image.

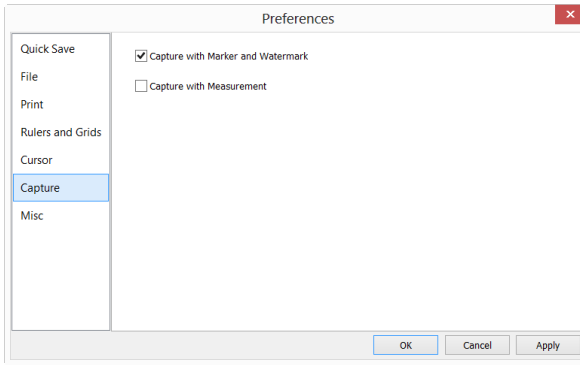

## 16.1.7 Misc Page

The **Misc** page is mainly used for the control of the **ImageView** UI. It mainly includes:

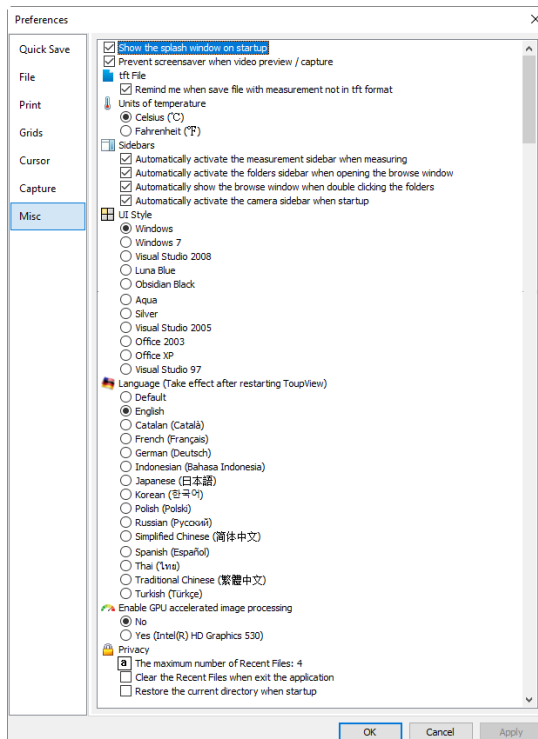

1. **ImageView'** special file format warning information;
2. Units of temperature
3. Sidebars;
4. UI Style;
5. Language;
6. Privacy;

settings et al.

## 16.2 Measurements(M)●●●

This sheet has many pages. They are:


### 16.2.1 General page

The **General** page is shown below:

**The calculation results keep:** The combo box allows you to set the calculation results accuracy among 1decimal and 6 decimals. Default is **2 decimals**;

**Label font size:** The **Label** is used to display the **Objects** dimensions. the **Label font size** is among 5 and 15; Default is 15;


**Label Color:** The Label Font color for the **Objects** dimensions; Default is red;

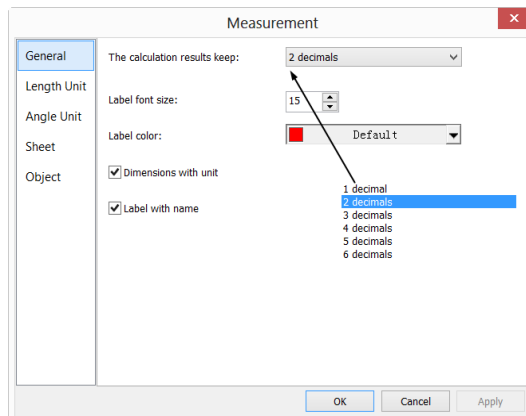

**Dimensions with unit:** If this box is checked, the **Dimension** will be displayed together with the unit for the **Objects**. If unchecked, only the **Dimension** will be displayed with the **Objects**.

## Options

**Label with name:** Checking **Label with name** will add a **Prefix** before the **Objects** number. The **Prefix** for the different **Object** can be specified in the Measurement Sidebar where there is an item called: **Name**. Here, we show an example for **Line Object** with and without **Prefix L1** as below:

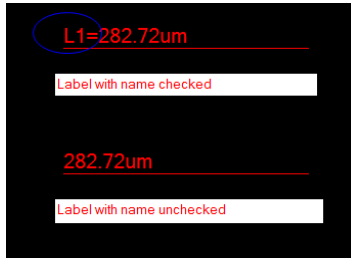

### 16.2.2 Length Unit page



**Length Unit page:** One can select the **Length Unit** for the **Measurements** menu's **Objects** on the **Layer Measurement** operation.

**Unit:** The system unit defined by the **ImageView**. It cannot be deleted;

**Current:** The **Unit** selected or checked;

**Type:** Type of unit. It can be **System** (Defined by **ImageView**) or **User** (Defined by the user) type;

**Scale:** Represents the ratio of "Meter by unit". For example, if the unit is  $\mu\text{m}$ , then "Meter by  $\mu\text{m}$ " should be 1000000, the **Scale** should be  $1\text{e}+6$ ;

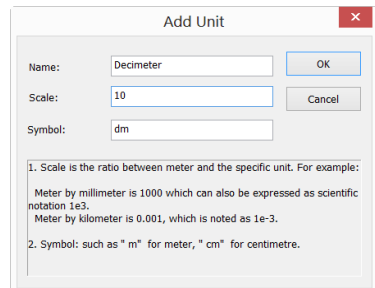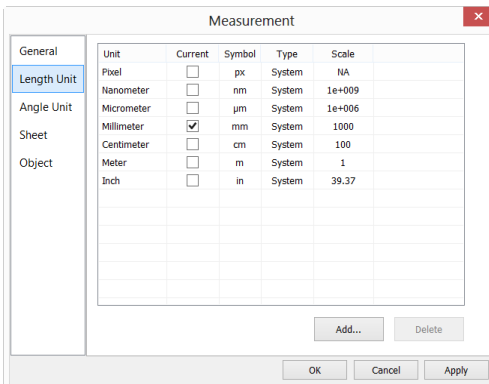


**Add:** User can also define his own **Unit**. Clicking **Add...** button and the **Add Unit**

## Options

dialog will be brought up as above;

Here, one can enter the unit **Name** and **Symbol** in their fields. Here, we enter a name called **Decimeter** and its **Symbol** is **dm**, its **Scale** for **Meter** by **Decimeter** is 10. Click **OK** to end the **Add Unit** operation, or **Cancel** to cancel the **Add Unit** operation.


The final **Length Unit** list looks like the figure below:

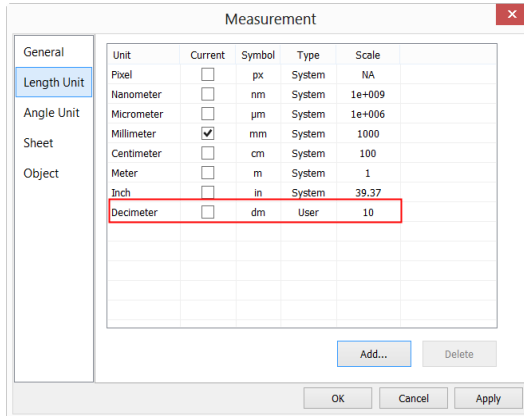

You can find the **Type** is now named **User**. This means that this **Unit** is not defined by the **System**, but by the **User**.

### 16.2.3 Angle Unit page

On the **Angle Unit** page, one can select **Radian**, **Degree**, or **PI** as the **Angle Unit**.

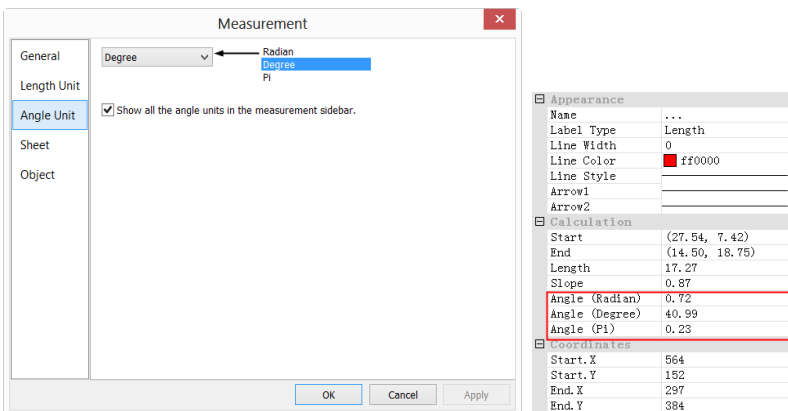

Show all the angle units in the measurement sidebar will list all the Object Units in the Measurement Sidebar as shown above for reference.

### 16.2.4 Sheet page

See the [View>Measurement Sheet](#) menu to understand its functions.


1. To modify the Measurement Sheet's item order, click the item to highlight it, the Up or Down buttons will be enabled (If the item is in the third position, the Up button will be disabled, if the item is in the last position, the Down button will be disabled). Click the Up or Down buttons to modify the item position;

**Note:** The item Index and Name are always in grayed states, this means these two items cannot be modified (Both their hide/show states and their positions).

2. Checking/Unchecking the item will show/hide the item in the Measurement Sheet;

3. Clicking Default will return to the ImageView's default settings;


4. Both the name and order for Item 1(Index) and item 2(Name) cannot be changed.

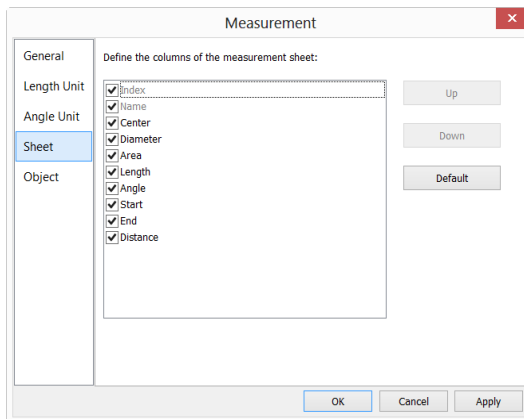

### 16.2.5 Object page

The Object page list the Point, Line, Parallel, Two Parallels, Vertical, Angle, Rectangle, Circle, Arc, Annulus, Two Circles, Ellipse, Polygon, Scale Bar, Text characteristics. Their characteristics can be modified in this page according to the requirement. Different Object has different characteristics.

## Options

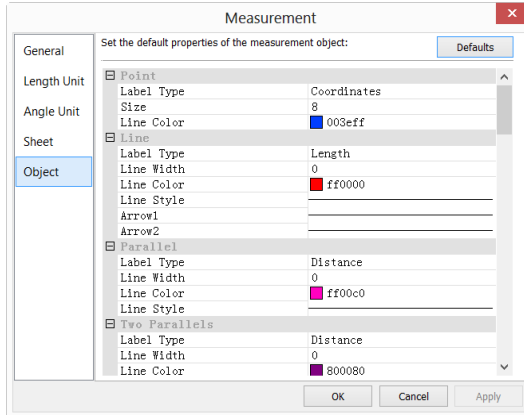


Click [Defaults](#) can return the all the modifications to the [Default](#) one.

### 16.3 Magnifications(F)●●●

Choose the [Options>Magnification●●●](#) command to manage the calibrated [Magnification](#).

If one has defined the 4x, 10X, 40X, 100X [Magnifications](#), the [Magnification](#) dialog should look like:

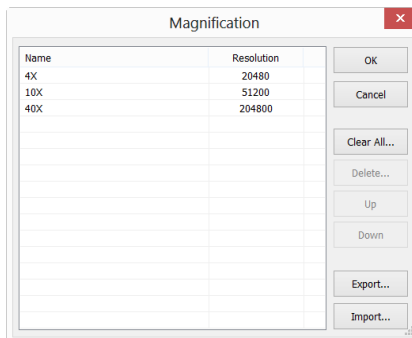


1. Highlight the [Magnification](#) item and the [Delete●●●](#) button will be enabled. Click [Delete●●●](#) to delete the selected item;
2. Highlight the [Magnification](#) item, click the [Up](#) or [Down](#) button to modify the [Magnification](#) list order; The [Up](#) or [Down](#) button will be disabled when the highlight item is at the first or last position;


3. Click **Clear All...** to delete all of the **Magnification** items; If one wishes to use the **Magnification** late, a backup should be made first;
4. Click **Export...** to back up the **Magnification** in a safe media. The file extension is **".magn"**;
5. After the new installation is finished, the **Magnification** can be import by choosing the **Options>Magnification...** command and click **Import...** to load the previously saved **".magn"** file;
6. If everything is ok, press **OK** to end the **Magnification** management dialog.


### 16.4 Calibrate(D)...



The detailed calibration steps are as follows:


1. Run **ImageView**;
2. Connect the camera to the computer and microscope;
3. Start the camera (Here, it is **XXXXX**);
4. Switch the microscope object to 10X and put the TS-M1 micrometer in the middle of the microscope field and try to find the ruler clearly. Set the **Unit** to **Pixel** and the video **Resolution** to the maximum one (2048X1534 for **XXXXX**) and **Zoom** ratio to 100% (see );

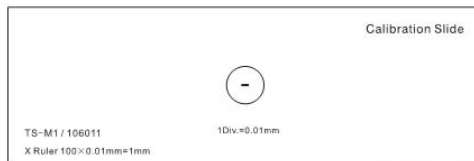


5. Choosing the **Options>Calibrate...** command or clicking "" on the toolbar, a red line with pixels number and 0.000um length is overlaid on the video window. At the same time, a dialog called **Calibrate** will be displayed over the video window;



## Options

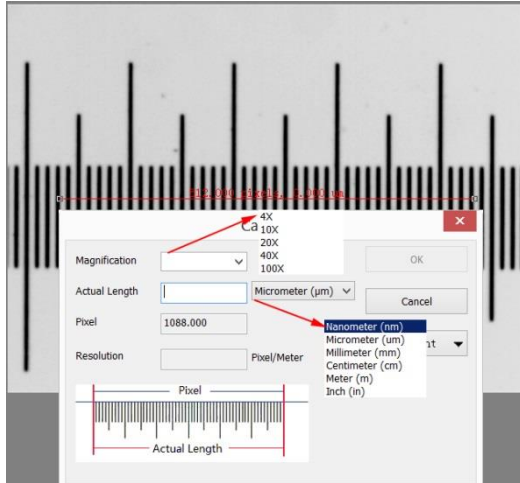



6. Try to align the two ends of the red line with the video ruler scale (Try to pull the red line as long as possible to keep the calibration accuracy);
7. Enter or select the current microscope objective lens **Magnification** in the **Magnification** field. The current **Magnification** is 10X;
8. Read the overlaid (by the red line) micro-ruler actual length and fill it in the **Actual Length** field, the current **Actual Length** is 450µm. This **Actual Length** will also be displayed in the middle of the red line just behind the pixel number. At the same time, the **Resolution** will be calculated and displayed simultaneously in the **Resolution** field.

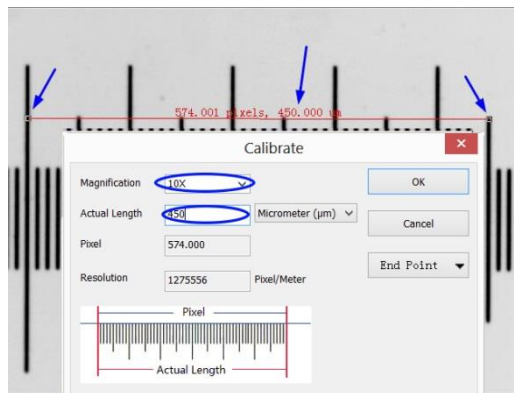


## Options


9. If everything is ok, click **Ok** to end the calibration. The **Magnification** 10X (This is the number you entered in the **Magnification** edit box) will be available in the

**Magnification** dropdown combobox on the video window toolbar ;


10. If you wish to make the measurement under this **Magnification**, choose 10X in the above **Magnification** dropdown combobox first and then choose **Unit** in the **Unit** dropdown list box(  ) which is just in the left of the **Magnification**'s dropdown combobox (User can also choose **Unit** through the **Option>Measurements...** menu, a dialog called **Measurement** will be brought up. Click **Length Unit** page to display the **Length Unit** page and checking **Unit** in the **Current** item.

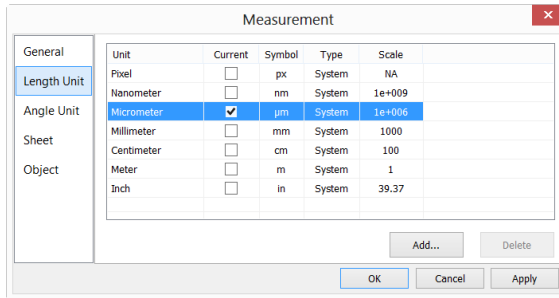

Now, you can measure the objects with the selected **Unit** at ease.




11. The selected **Resolution** can be saved for the future image **Measurement** operations. If the **Measurements** are performed on the video, the objects and **Resolution** can be saved in the image with **ImageView File Format (\*.tff)** for the future applications;

12. The other microscope **Magnification** such as 4X, 40X, 100X can also be defined just as the above steps. Thus when you switch the microscope objective lens, you just need to select the **Magnification** ( for example) on the toolbar to perform

the [Measurement](#) operations.

### 16.5 Edit Dye List(E)●●●

The [Dye List](#) can be used for the [Process>Color Composite](#) operation. The new [Dye List](#) feature in [ImageView](#) allows you to select from a list of dyes, or add your custom dyes to the list. The list of dyes ([ImageView.dye](#)) is stored under [C:\Program Files\ToupTek\ImageView](#) directory.

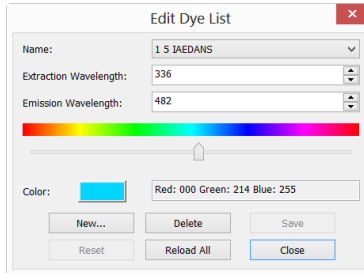


When you choose [Options>Edit Dye List●●●](#) command, you will see the [Edit Dye List](#) dialog box:

The list includes any dye definitions found in the current location. When this feature is used to prompt for a specific dye, the list indicates the currently selected dye, or you may select a dye from the drop-down list.

**Name:** This list includes all dye definitions found in the current dye file. You may select a different dye from the drop-down list, and all the remaining controls will be updated to show the characteristics of the new dye.


**Emissions Wavelength:** This field displays the emissions wavelength for the dye you have chosen. You can adjust the emissions wavelength by entering a new value. The default color will change in response to changes in the emissions wavelength.

**Excitation wavelength:** The default wavelength for your dye is displayed here. You can adjust the wavelength by entering a new value.


**Color:** Use the slider to adjust the emissions wavelength for your dye, which also sets the default display color. (You can also use the [Color](#) button  to select a specific color using a standard Windows color selection dialog) The color will change in

## Options

response to changes in the emissions wavelength. Here you can change the color associated with the selected dye, or define a custom color. The color default is linked to the selection of a wavelength for your dye. If you change the [Emissions Wavelength](#), the color displayed will be the standard color for that wavelength. To set a custom color, first you should set the wavelength and then edit the color.

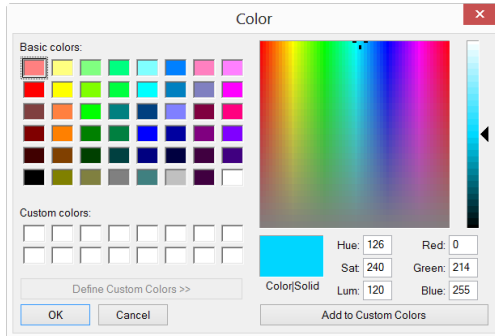

**New:** Clicking [New](#) will setup a new dye, this will invoke a dialog called [New Dye](#). Input your [New Dye](#) name and click [Ok](#) to end the dialog and click [Cancel](#) to cancel the input. This will return to the [Edit Dye List](#) again and the new name will be the default on in the Name list box. Try to set the [Emissions wavelength](#), [Excitation wavelength](#), [Color](#) for your new dye.

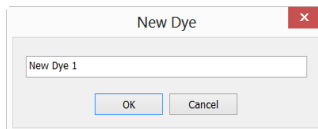

**Save:** Click [Save](#) on [Edit Dye List](#) to save your dye selection


**Close:** Click the [Close](#) button to end the [Edit Dye List](#) dialog:

### 16.6 Auto Correction(A)●●●

Set the low and high ranges for the [Image>Adjust>Auto Level](#) and [Image>Adjust>Auto Contrast](#) menus. The default value is 0.5% for both, but [ImageView](#) suggests this value be smaller than 1%.

## Options

---



See [Image>Adjust>Auto Level](#) and [Image>Adjust>Auto Contrast](#) for details.


## 17 Window

### 17.1 Close All(C)


Choosing the **Closes All** command to close all of the pictures opened or captured inside **ImageView** frame. If you have made any modifications to the pictures or if you have captured some pictures from the camera, choosing the **Close All** will let you finish the saving operations quickly.



If the above image windows exist, choosing the **Window>Close All** command will bring up a **Save Files** dialog as below:

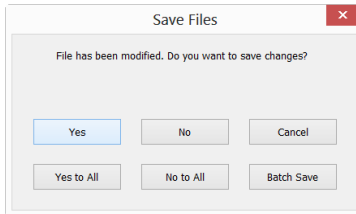

1. Clicking **Yes** on the **Save Files** dialog will close the **Video** , **Browse**, **Image** windows directly that are not changed without ask anything. If there are newly created **Image** windows, **ImageView** will bring up a **Save As** dialog to prompt user to enter the **File name** to save file.

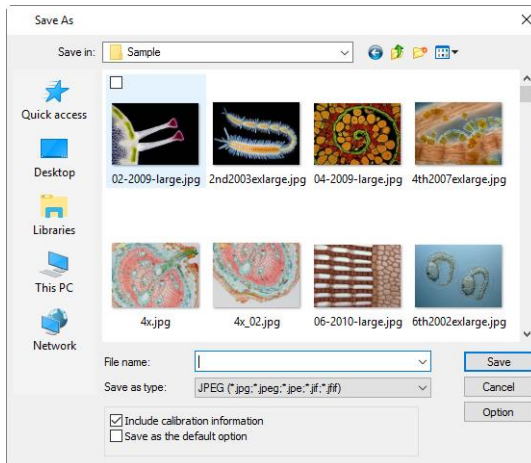


If **Save** or **Cancel** is clicked in the **Save As** dialog, **ImageView** will return to the **Save Files** dialog to continue the next file close operation;

2. Clicking **No** on **Save Files** dialog will close the current image window without saving operation and return to the **Save Files** dialog to continue the next file operation;
3. Clicking **Cancel** will cancel the **Save Files** dialog without doing anything;
4. Clicking **Yes to All** on **Save Files** dialog will always bring up a **Save As** dialog to let you enter the **File name** to save files one by one until all of the files are saved;
5. Clicking **No to All** on **Save Files** dialog will close all of the image windows without saving them;
6. Clicking **Batch Save** on **Save Files** dialog will transfer the save process to **File>Batch Save...** command. Please check the **File>Batch Save...** menu for details;

**Note:** If you have a lot of pictures opened and have made some modifications on them and want to close them quickly without saving anything, you may use this command and choose Step 5. All the images will be closed instantly, no warning will be given.

### 17.2 Reset Window Layout(R)

Choosing **Window>Reset Window Layout** will reset the **ImageView** window layout to the original one. The reset will be effective after restart.

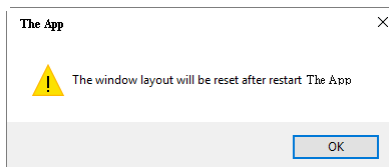

### 17.3 Windows(W)...




Choosing the **Window>Windows...** will open a dialog box that lets you manage the currently opened windows.

The dialog allows you to manage large lists of open windows by assigning them into


## Window

---

groups. Let us say you have 10 windows opened, but want to close 4 of them scattered through the list.

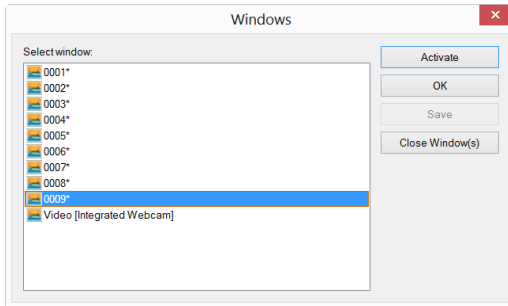

1. Choose the [Window>Windows...](#) command;
2. Select the windows you want to close. Hold **Ctrl** or **Shift** key to select more than one at a time. Here, 4 items are selected;

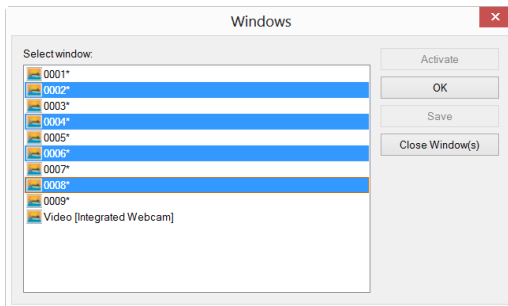

3. Click [Close Window\(s\)](#) button, those 4 selected windows will be closed, leaving the other files or captures available for editing;
4. User can use this command to switch to the checked window on a list by hitting [Activate](#) (or "bring up" from an icon multiple windows).



## 18 Help

### 18.1 Help Contents(H)



### F1

Choose the [Help>Help Contents](#) command to load [ImageView](#) help file. The help file is in Portable Document Format (PDF).

PDF is a file format used to represent documents in a manner independent of application software, hardware, and operating systems. Each PDF file encapsulates a complete description of a fixed-layout flat document, including the text, fonts, graphics, and other information needed to display it. In 1991, Adobe Systems co-founder John Warnock outlined a system called "Camelot" that evolved into PDF.


While the PDF specification has been available free of charge since at least 2001, PDF was originally a proprietary format controlled by Adobe. It was officially released as an open standard on July 1, 2008, and published by the International Organization for Standardization as ISO 32000-1:2008. In 2008, Adobe published a Public Patent License to ISO 32000-1 granting royalty-free rights for all patents owned by Adobe that are necessary to make, use, sell and distribute PDF compliant implementations.

If your computer still does not install the PDF reader, please try to download it from:

<http://www.adobe.com/downloads/>

### 18.2 About(A)●●●

Display the related information about [ImageView](#), including [ImageView version](#), [Compatible](#), [Built](#) date and its developer's [www](#) etc.

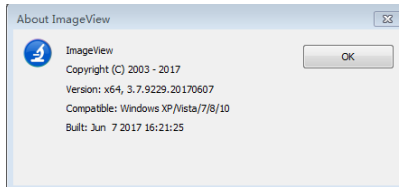

Clicking on the [URL](#) link will direct you to the address of the application supplier. If you have any problem with the camera or application, please feel free to contact your supplier.