

# TEST REPORT


Applicant: XIAMEN PROBTAIN MEDICAL TECHNOLOGY CO., LTD.  
NO. 6, JI'AN ROAD, TONG'AN DISTRICT  
XIAMEN CITY  
CHINA

Number: HKGH02595531 S1

Date: May 25, 2020

*This is to supersede Report No. HKGH02595531 dated May 25, 2020 due to information update*

Submitted sample said to be :  
Item Name : **Disposable Surgical Mask**  
Item No. : MP9017  
Specification : 17.5\*9.5cm  
Quantity : 100 pieces  
Manufacturer : XIAMEN PROBTAIN MEDICAL TECHNOLOGY CO., LTD.  
Sample Received Date : May 07, 2020  
Testing Period : May 07, 2020 to May 20, 2020

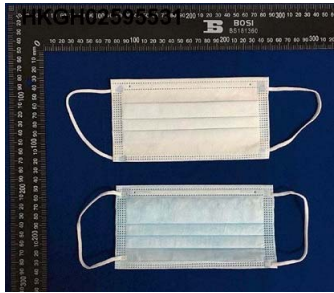

**Conclusion:**

The submitted sample was tested under the following requirements requested by the applicant, subject to the information stated in the remark and attached page(s) for details :

Requirement	Result
(1) Differential pressure [EN 14683:2019+AC:2019]	Pass
(2) Splash resistance pressure [EN 14683:2019+AC:2019]	Pass
(3) Bacterial filtration efficiency (BFE) [EN 14683:2019+AC:2019]	Pass
(4) Microbial cleanliness [EN 14683:2019+AC:2019]	Pass

For and on behalf of :  
Intertek Testing Services HK Ltd.

Cindy I.K. Chan  
Vice President



# TEST REPORT

Number : HKGH02595531 S1

(1) Differential pressure ^

Test Method: With reference to EN 14683:2019+AC:2019

Result:

Sample	Differential pressure (Pa/cm <sup>2</sup> )	Requirement (Pa/cm <sup>2</sup> )	Classification	Conclusion
1	32.7	$<60$ EN 14683:2019+AC:2019	Type II R	Pass
2	34.1			
3	33.3			
4	34.3			
5	33.5			

Remark :

^ = This is a subcontracting item

Date sample received : May 25, 2020

Testing period : May 07, 2020 to May 25, 2020

\*\*\*\*\*



# TEST REPORT

Number : HKGH02595531 S1

(2) Splash resistance pressure ^

Test Method: With reference to EN 14683:2019+AC:2019

Result:

Sample	Measured value	Requirement (kPa)	Classification	Conclusion
	Pressure			
	16.0 kPa			
1	pass	≥16.0 EN 14683:2019+AC:2019	Type II R	Pass
2	pass			
3	pass			
4	pass			
5	pass			
6	pass			
7	pass			
8	pass			
9	pass			
10	pass			
11	pass			
12	pass			
13	pass			
14	pass			
15	pass			
16	pass			
17	pass			
18	pass			



# TEST REPORT

Number : HKGH02595531 S1

Sample	Measured value	Requirement (kPa)	Classification	Conclusion
	Pressure			
19	pass			
20	pass			
21	pass			
22	pass			
23	pass			
24	pass			
25	pass			
26	pass			
27	pass			
28	pass			
30	pass			
31	pass			
32	pass			
Final result	pass			

**Remark :**

An acceptable quality limit of 4.0% is met for a single sampling plan when 29 or more of the 32 tested specimens show "pass" results.

^ = This is a subcontracting item

Date sample received : May 25, 2020

Testing period : May 07, 2020 to May 25, 2020

\*\*\*\*\*



# TEST REPORT

Number : HKGH02595531 S1

(3) Bacterial Filtration Efficiency (BFE) ^

Test Method: With reference to EN 14683:2019+AC:2019

Dimensions of the test specimens : 175 mm x 175 mm

Result:

Sample	BFE (%)	Requirement (%)	Classification	Conclusion
1	100	$\geq 98$ EN 14683:2019+AC:2019	Type II R	Pass
2	100			
3	100			
4	100			
5	100			

Remark :

^ = This is a subcontracting item

Date sample received : May 25, 2020

Testing period : May 07, 2020 to May 25, 2020

\*\*\*\*\*



# TEST REPORT

Number : HKGH02595531 S1

(4) Microbial cleanliness ^

Test Method: With reference to EN 14683:2019+AC:2019

Result:

Sample	Microbial cleanliness (CFU/g)	Requirement (CFU/g)	Classification	Conclusion
1	2	≤30 EN 14683:2019+AC:2019	Type II R	Pass
2	1			
3	2			
4	0			
5	0			

Remark :

^ = This is a subcontracting item

Date sample received : May 25, 2020

Testing period : May 07, 2020 to May 25, 2020

\*\*\*\*\*

End of report

*This report is for the exclusive use of Intertek's Client and is provided pursuant to the agreement between Intertek and its Client. Intertek's responsibility and liability are limited to and subject to our standard Terms and Conditions which can be obtained at our website: <http://www.intertek.com/terms/>. Intertek assumes no liability to any party, other than to the Client in accordance with the agreement, for any loss, expense or damage occasioned by the use of this report. Intertek is responsible for all the information provided in the reports, except when information is provided by the Client or when the Client requires the item to be tested acknowledging a deviation from specified conditions that can affect the validity of results.*

*The observations and test results in this report are relevant to the sample(s) tested and submitted by client. The report is not intended to be a recommendation for any particular course of action, you are responsible for acting as you see fit on the basis of the report results. This report does not discharge or release you from your legal obligations and duties to any other person. Only the Client is authorized to permit copying or distribution of this report and the report shall not be reproduced except in full. Any use of the Intertek name or one of its marks for the sale or advertisement of the tested material, product or service must first be approved in writing by Intertek. This report by itself does not imply that.*



To: XIAMEN PROBTAIN MEDICAL  
TECHNOLOGY CO., LTD.

Ref: FC-2020-3708

Attention:

Date: Jun 02, 2020

---

Re : Report Revision Notification

Intertek Testing Services Report Number HKGH02595531 Dated May 25, 2020

Please be informed that all the content recorded in the above captioned report will be void. This captioned report is now superseded by a revised Intertek Testing Services report, HKGH02595531 S1

Thank you for your attention.

For and on behalf of :  
Intertek Testing Services HK Ltd.



Cindy I.K. Chan  
Vice President